




TEST REPORT

Reference No..... : WTX21X09095480E-1
 Applicant : GlobTek, Inc.
 Address : 186 Veterans Dr. Northvale, NJ 07647 USA
 Product : Medical/ITE Power Supply
 Test Model : GTM96180-1811-2.0-T3, GTM91120-3024-T3A, GTM96300-3624-T2
 Standards : EN 55032:2015+A11:2020
 EN 55035:2017+A11:2020
 EN IEC 61000-3-2:2019
 EN 61000-3-3:2013+A1:2019
 Date of Receipt sample : Oct. 19, 2021
 Date of Test..... : Oct. 20, 2021 to Nov. 25, 2021
 Date of Issue : Nov. 25, 2021
 Test Result..... : Pass

Remarks:

The results shown in this test report refer only to the sample(s) tested, this test report cannot be reproduced, except in full, without prior written permission of the company. The report would be invalid without specific stamp of test institute and the signatures of compiler and approver.



Prepared By:

Waltek Testing Group (Shenzhen) Co., Ltd.

Address: 1/F., Room 101, Building 1, Hongwei Industrial Park, Liuxian 2nd Road,
Block 70 Bao'an District, Shenzhen, Guangdong, China

Tel.: +86-755-33663308

Fax.: +86-755-33663309

Tested by:

Reviewed By:

Approved & Authorized By:

Dace Huang/Project Engineer

Evan Cai / EMC Manager

Silin Chen / Manager



TABLE OF CONTENTS

| | |
|----------------------------------------------------------------------|-----------|
| 1. GENERAL INFORMATION..... | 4 |
| 1.1 PRODUCT DESCRIPTION FOR EQUIPMENT UNDER TEST (EUT)..... | 4 |
| 1.2 TEST STANDARDS..... | 7 |
| 1.3 TEST METHODOLOGY..... | 7 |
| 1.4 EUT SETUP AND OPERATION MODE..... | 8 |
| 1.5 PERFORMANCE CRITERIA FOR EMS..... | 9 |
| 1.6 TEST EQUIPMENT LIST AND DETAILS..... | 10 |
| 2. SUMMARY OF TEST RESULTS..... | 11 |
| 3. CONDUCTED EMISSION..... | 12 |
| 3.1 MEASUREMENT UNCERTAINTY..... | 12 |
| 3.2 BASIC TEST SETUP BLOCK DIAGRAM..... | 12 |
| 3.3 ENVIRONMENTAL CONDITIONS..... | 13 |
| 3.4 SUMMARY OF TEST RESULTS..... | 13 |
| 4. RADIATED EMISSION..... | 20 |
| 4.1 MEASUREMENT UNCERTAINTY..... | 20 |
| 4.2 BASIC TEST SETUP BLOCK DIAGRAM..... | 20 |
| 4.3 CORRECTED AMPLITUDE & MARGIN CALCULATION..... | 21 |
| 4.4 ENVIRONMENTAL CONDITIONS..... | 21 |
| 4.5 SUMMARY OF TEST RESULTS..... | 21 |
| 5. HARMONIC CURRENT EMISSIONS..... | 28 |
| 5.1 TEST PROCEDURE..... | 28 |
| 5.2 TEST STANDARDS..... | 28 |
| 5.3 ENVIRONMENTAL CONDITIONS..... | 28 |
| 5.4 BASIC TEST SETUP BLOCK DIAGRAM..... | 28 |
| 5.5 HARMONIC CURRENT EMISSIONS TEST DATA..... | 28 |
| 6. VOLTAGE FLUCTUATION FLICKER..... | 29 |
| 6.1 TEST PROCEDURE..... | 29 |
| 6.2 TEST STANDARDS..... | 29 |
| 6.3 ENVIRONMENTAL CONDITIONS..... | 29 |
| 6.4 BASIC TEST SETUP BLOCK DIAGRAM..... | 29 |
| 6.5 VOLTAGE FLUCTUATION AND FLICKER TEST DATA..... | 29 |
| 7. ELECTROSTATIC DISCHARGES (ESD)..... | 33 |
| 7.1 TEST PROCEDURE..... | 33 |
| 7.2 TEST PERFORMANCE..... | 33 |
| 7.3 ENVIRONMENTAL CONDITIONS..... | 33 |
| 7.4 BASIC TEST SETUP BLOCK DIAGRAM..... | 33 |
| 7.5 ELECTROSTATIC DISCHARGE IMMUNITY TEST DATA..... | 34 |
| 8. CONTINUOUS RF ELECTROMAGNETIC FIELD DISTURBANCES (RS)..... | 35 |
| 8.1 TEST PROCEDURE..... | 35 |
| 8.2 TEST PERFORMANCE..... | 35 |
| 8.4 BASIC TEST SETUP BLOCK DIAGRAM..... | 35 |
| 8.5 CONTINUOUS RADIATED DISTURBANCES TEST DATA..... | 36 |
| 9. ELECTRICAL FAST TRANSIENTS (EFT)..... | 37 |
| 9.1 TEST PROCEDURE..... | 37 |
| 9.2 TEST PERFORMANCE..... | 37 |
| 9.4 BASIC TEST SETUP BLOCK DIAGRAM..... | 37 |
| 9.5 ELECTRICAL FAST TRANSIENTS TEST DATA..... | 38 |
| 10. SURGES..... | 40 |
| 10.1 TEST PROCEDURE..... | 40 |
| 10.2 TEST PERFORMANCE..... | 40 |
| 10.4 BASIC TEST SETUP BLOCK DIAGRAM..... | 40 |



| | |
|-----------------------------------------------------------|-----------|
| 10.5 SURGE TEST DATA..... | 41 |
| 11. CONTINUOUS INDUCED RF DISTURBANCES (C/S) | 42 |
| 11.1 TEST PROCEDURE | 42 |
| 11.2 TEST PERFORMANCE | 42 |
| 11.3 ENVIRONMENTAL CONDITIONS..... | 42 |
| 11.4 BASIC TEST SETUP BLOCK DIAGRAM | 42 |
| 11.5 CONTINUOUS CONDUCTED DISTURBANCES TEST DATA | 43 |
| 12. POWER-FREQUENCY MAGNETIC FIELDS (PFMF) | 44 |
| 12.1 TEST PROCEDURE | 44 |
| 12.2 TEST PERFORMANCE | 44 |
| 12.3 ENVIRONMENTAL CONDITIONS..... | 44 |
| 12.4 BASIC TEST SETUP BLOCK DIAGRAM | 44 |
| 12.5 POWER-FREQUENCY MAGNETIC FIELD TEST DATA | 45 |
| 13. VOLTAGE DIPS AND INTERRUPTIONS..... | 46 |
| 13.1 TEST PROCEDURE | 46 |
| 13.2 TEST PERFORMANCE | 46 |
| 13.3 ENVIRONMENTAL CONDITIONS..... | 46 |
| 13.4 BASIC TEST SETUP BLOCK DIAGRAM..... | 46 |
| 13.5 VOLTAGE DIPS AND INTERRUPTIONS TEST DATA | 47 |
| EXHIBIT 1 - PRODUCT LABELING | 48 |
| PROPOSED CE LABEL FORMAT | 48 |
| PROPOSED LABEL LOCATION ON EUT | 48 |
| EXHIBIT 2 - EUT PHOTOGRAPHS..... | 49 |
| EXHIBIT 3 - TEST SETUP PHOTOGRAPHS | 60 |

WALTEK




1. GENERAL INFORMATION

1.1 Product Description for Equipment Under Test (EUT)

Client Information

Applicant: GlobTek, Inc.
 Address of applicant: 186 Veterans Dr. Northvale, NJ 07647 USA

Manufacturer: 1. GlobTek, Inc.
 2. GlobTek (Suzhou) Co., Ltd
 Address of manufacturer: 1.186 Veterans Dr. Northvale, NJ 07647 USA
 2. Building 4, No. 76, Jin Ling East Rd., Suzhou Industrial Park, Suzhou, JiangSu 215021, China

| General Description of EUT | |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------|
| Product Name: | Medical/ITE Power Supply |
| Trade Name: |  |
| Model No.: | GTM96180-1811-2.0-T3, GTM91120-3024-T3A, GTM96300-3624-T2 |
| Adding Model(s): | / |
| <p><i>Note: The test data is gathered from a production sample, provided by the manufacturer.</i></p> <p><i>GT*96180-*****, GT*96300-*****, GT*91120-*****,</i></p> <p><i>GT*96180-*****,</i></p> <p><i>The 1st "*" part can be 'M' or '-' or 'H' for market identification and not related to safety.</i></p> <p><i>The 2nd "*" denotes the rated output wattage designation, which can be "01" to "18", with interval of 1.</i></p> <p><i>The 3rd "*" denotes the standard rated output voltage designation, which can be "07", "11", "17.9", "30", "38", "48", "54" or "56";</i></p> <p><i>The 4th "*" is optional deviation, subtracted from standard output voltage, which can be "-0.01" to "-12.0" with interval of 0.01, or blank to indicate no voltage different.</i></p> <p><i>The 3rd "*" and 4th "*" together denote the output voltage, with a range of 5 - 56 volts.</i></p> <p><i>The 5th "*" = blank, it means wall plug in with interchangeable blade</i></p> <p><i>=-T2 means desktop class II with C8 AC inlet</i></p> <p><i>=-T2A means desktop class II with C18 AC inlet</i></p> <p><i>=-T3 means desktop class I or class II with functional earth with C14 AC inlet</i></p> <p><i>=-T3A means desktop class I or class II with functional earth with C6 AC inlet</i></p> <p><i>The 6th "*" = Blank or -AP or -PP or -SP</i></p> <p><i>-AP (with baby board) stands for Active POE (full IEEE compliant)</i></p> <p><i>-PP (no baby board) stands for Passive POE</i></p> <p><i>-SP (no baby board) stands for Simple POE</i></p> | |



*The last * denote any six character = 0-9 or A-Z or ()[] or – or blank for marketing purposes.*

Ratings

When the 6th “” is blank:*

*GT*96180-*****, Input: 100-240V~, 50-60Hz or 50/60Hz, 0.6A, Output: 5-48Vdc, Max. 3.6A, Max. 18W*

When the 6th “” = -AP or -PP or -SP:*

*GT*96180-*****, Input: 100-240V~, 50-60Hz or 50/60Hz, 0.6A, Output: 18-56Vdc, Max. 1.0A, Max. 18W*

*GT*96300-***** and GT*91120-******

The 1st “” part can be ‘M’ or ‘-’ or ‘H’ for market identification and not related to safety.*

The 2nd “” denotes the rated output wattage designation, which can be “01” to “36”, with interval of 1.*

The 3rd “” denotes the standard rated output voltage designation, which can be “07.5”, “10.5”, “14.5”, “19.5”, “24”, “36”, “48”, “54” or “56”;*

The 4th “” is optional deviation, subtracted from standard output voltage, which can be “-0.01” to “-11.9” with interval of 0.01, or blank to indicate no voltage different.*

The 3rd “” and 4th “*” together denote the output voltage, with a range of 5 - 56 volts.*

The 5th “” = -T2 means desktop class II with C8 AC inlet*

= -T2A means desktop class II with C18 AC inlet

= -T3 means desktop class I or class II with functional earth with C14 AC inlet

= -T3A means desktop class I or class II with functional earth with C6 AC inlet

= -R2 means hybrid desktop housing class II with C8 AC inlet

= -R3A means hybrid desktop housing class I or class II with functional earth with C6 AC inlet

= -F means Open Frame class I or class II with functional earth

= -FW means Open Frame class II

= -P2 means Encapsulated class II

= -P3 means Encapsulated class I or class II with functional earth

The 6th “” = Blank or -AP or -PP or -SP*

-AP (with baby board) stands for Active POE (full IEEE compliant)

-PP (no baby board) stands for Passive POE

-SP (no baby board) stands for Simple POE

*The last * denote any six character = 0-9 or A-Z or ()[] or – or blank for marketing purposes.*

Ratings

When the 6th “” is blank:*

*GT*96300-*****, Input: 100-240V~, 50-60Hz or 50/60Hz, 1.0A, Output: 5-48Vdc, Max. 4.5A, Max. 36W*

*GT*91120-*****, Input: 100-240V~, 50-60Hz or 50/60Hz, 1.5A, Output: 5-48Vdc, Max. 4A, Max. 30W*

When the 6th “” = -AP or -PP or -SP:*

*GT*96300-*****, Input: 100-240V~, 50-60Hz or 50/60Hz, 1.0A, Output: 18-56Vdc, Max. 2.0A, Max. 36W*

Technical Characteristics of EUT



| | |
|------------------------------|---------------------|
| Rated Voltage: | AC 100-240V 50-60Hz |
| Rated Current: | / |
| Rated Power: | / |
| Power Adaptor Model: | / |
| Highest Internal Frequency: | Below 108MHz |
| Classification of Equipment: | Class B |

WALTEK



1.2 Test Standards

The tests were performed according to following standards:

EN 55032:2015+A11:2020: Electromagnetic compatibility of multimedia equipment - Emission requirements.

EN 55035:2017+A11:2020: Electromagnetic compatibility of multimedia equipment - Immunity requirements.

EN IEC 61000-3-2:2019: Electromagnetic compatibility (EMC) -- Part 3-2: Limits - Limits for harmonic current emissions (equipment input current up to and including 16 A per phase).

EN 61000-3-3:2013+A1:2019: Electromagnetic compatibility (EMC) -- Part 3-3: Limits - Limitation of voltage changes, voltage fluctuations and flicker in public low-voltage supply systems, for equipment with rated current ≤ 16 A per phase and not subject to conditional connection.

Maintenance of compliance is the responsibility of the manufacturer. Any modification of the product maybe which result in lowering the emission/immunity should be checked to ensure compliance has been maintained.

1.3 Test Methodology

All measurements contained in this report were conducted with the standards EN 55032, EN IEC 61000-3-2, EN 61000-3-3 and EN 55035 for electromagnetic compatibility of multimedia equipment, and all related testing and measurement techniques intentional standards.



1.4 EUT Setup and Operation Mode

The equipment under test (EUT) was configured to measure its highest possible emission/immunity level. The test modes were adapted according to the operation manual for use, more detailed description as follows:

| Test Mode List | | | |
|----------------|--------------|----------------------------------------------|-------------------|
| Test Mode | Description | Remark | Power Supply Mode |
| TM1 | Working mode | Maximum power mode (GTM96180-1811-2.0-T3) | AC 230V/50Hz |
| TM2 | Working mode | Maximum power mode (GTM91120-3024-T3A) | AC 230V/50Hz |
| TM3 | Working mode | Maximum power mode (GTM96300-3624-T2) | AC 230V/50Hz |

Note: The product was measured at two nominal voltages of 230V and 110V, using a frequency of 50Hz or 60Hz. This report shows the worst case with 230V/50Hz data.

| EUT Cable List and Details | | | | |
|----------------------------|------------|---------------------|------------------------|---------------------|
| Cable Description | Length (m) | Shielded/Unshielded | With / Without Ferrite | With / Without Chip |
| Cable (GT96180) | 2.5 | Unshielded | With | Without |
| Cable (GT91120) | 2.5 | Unshielded | With | Without |
| Cable (GT96300) | 1.8 | Unshielded | Without | Without |

| Special Cable List and Details | | | | |
|--------------------------------|------------|---------------------|------------------------|---------------------|
| Cable Description | Length (m) | Shielded/Unshielded | With / Without Ferrite | With / Without Chip |
| / | / | / | / | / |

| Auxiliary Equipment List and Details | | | |
|--------------------------------------|--------------|-------|---------------|
| Description | Manufacturer | Model | Serial Number |
| / | / | / | / |



1.5 Performance Criteria for EMS

All the test data has been collected, reduced, and analyzed within this report in accordance with Immunity requires the following as specific performance criteria:

- A. The apparatus shall continue to operate as intended during and after the test. The manufacturer specifies some minimum performance level. The performance level may be specified by the manufacturer as a permissible loss of performance.
- B. The apparatus shall continue to operate as intended after the test. This indicates that the EUT does not need to function at normal performance levels during the test, but must recover. Again some minimal performance is defined by the manufacturer. No change in operating state or loss of data is permitted.
- C. Temporary loss of function is allowed. Operation of the EUT may stop as long as it is either automatically reset or can be manually restored by operation of the controls.

WALTEK



1.6 Test Equipment List and Details

| Description | Manufacturer | Model | Serial No. | Cal. Date | Due. Date |
|------------------------------------|-----------------------|-----------------|----------------|------------|------------|
| Spectrum Analyzer | Rohde & Schwarz | FSP | 836079/035 | 2021-03-30 | 2022-03-29 |
| EMI Test Receiver | Rohde & Schwarz | ESVB | 825471/005 | 2021-04-12 | 2022-04-11 |
| Amplifier | Agilent | 8447F | 3113A06717 | 2021-04-12 | 2022-04-11 |
| Amplifier | C&D | PAP-1G18 | 2002 | 2021-04-12 | 2022-04-11 |
| Trilog Broadband Antenna | Schwarz beck | VULB9163 | 9163-333 | 2021-03-20 | 2023-03-19 |
| Horn Antenna | ETS | 3117 | 00086197 | 2021-03-19 | 2023-03-18 |
| Loop Antenna | Schwarz beck | FMZB 1516 | 9773 | 2021-03-20 | 2023-03-19 |
| EMI Test Receiver | Rohde & Schwarz | ESPI | 101391 | 2021-05-06 | 2022-05-05 |
| Trilog Broadband Antenna | Schwarz beck | VULB9163(B) | 9163-635 | 2021-04-09 | 2023-04-08 |
| Amplifier | Agilent | 8447D | 2944A10179 | 2021-04-12 | 2022-04-11 |
| EMI Test Receiver | Rohde & Schwarz | ESPI | 101611 | 2021-04-12 | 2022-04-11 |
| Pulse Limiter | Rohde & Schwarz | ESH3-Z2 | 100911 | 2021-04-15 | 2022-04-14 |
| AC LISN | Schwarz beck | NSLK8126 | 8126-224 | 2021-04-12 | 2022-04-11 |
| 8-WIRE LISN | Schwarz beck | 8158 | CAT3-8158-0059 | 2021-04-12 | 2022-04-11 |
| 8-WIRE LISN | Schwarz beck | 8158 | CAT5-8158-0117 | 2021-04-12 | 2022-04-11 |
| PMF Generator | LIONCEL | PMF-801C-C | 0171101 | 2021-04-12 | 2022-04-11 |
| PMF Antenna | LIONCEL | PMF-801C-A | 0180302 | 2021-04-12 | 2022-04-11 |
| Instantaneous PMF Generator Module | LIONCEL | PMF-801C-T | 0171001 | 2021-04-12 | 2022-04-11 |
| Digital Power Analyzer | California Instrument | CTS | 72831 | 2021-04-12 | 2022-04-11 |
| Power Source | California Instrument | 5001IX-CTS-400 | 25965 | 2021-04-12 | 2022-04-11 |
| ESD Generator | LIONCEL | ESD-203B | 0170901 | 2021-04-16 | 2022-04-15 |
| Transient 2000 | EMC PARTNER | TRA2000 | 863 | 2021-04-12 | 2022-04-11 |
| Couple Clamp | EMC PARTNER | CN-EFT1000 | 513 | 2021-04-12 | 2022-04-11 |
| CONDUCTED IMMUNITY TEST SYSTEM | FRANKONIA | CIT-10/75 | 126B1247/2013 | 2021-01-08 | 2022-01-07 |
| CDN | LIONCEL | CDN-T8 | 0210401 | 2021-05-06 | 2022-05-05 |
| Attenuator | EMTEST | MA-5100/6BF2 | 1009 | 2021-03-30 | 2022-03-29 |
| CDN | Luthi | L-801M2/M3 | 2665 | 2021-04-12 | 2022-04-11 |
| Signal Generator | HP | 8688B | 3438A00604 | 2021-03-30 | 2022-03-29 |
| Power Meter | KEITHLEY | 3500 | 1162591 | 2021-03-27 | 2022-03-26 |
| Power Meter | KEITHLEY | 3500 | 1121428 | 2021-03-27 | 2022-03-26 |
| RF Power Amplifier | MicoTop | MPA-80-1000-250 | MPA1906239 | 2021-03-27 | 2022-03-26 |
| RF Power Amplifier | MicoTop | MPA-80-1000-100 | MPA1906238 | 2021-03-27 | 2022-03-26 |
| Antenna | SCHWARZBECK | STLP 9129 | 9129 114 | N/A | N/A |



2. SUMMARY OF TEST RESULTS

| Standards | Description of Test Item | Result |
|------------------------------------------------|-------------------------------------------------------------------------------------------|-----------|
| EN 55032 | Conducted Emission | Compliant |
| | Radiated Emission | Compliant |
| EN IEC 61000-3-2 | Harmonic Current Emission | Compliant |
| EN 61000-3-3 | Voltage Fluctuation and Flicker | Compliant |
| EN 55035 | Electrostatic Discharge Immunity in accordance with EN 61000-4-2 | Compliant |
| | Continuous RF electromagnetic field Disturbances Immunity in accordance with EN 61000-4-3 | Compliant |
| | Electrical Fast Transient/Burst Immunity in accordance with EN 61000-4-4 | Compliant |
| | Surges Immunity in accordance with EN 61000-4-5 | Compliant |
| | Continuous induced RF disturbances Immunity in accordance with EN 61000-4-6 | Compliant |
| | Power-frequency Magnetic Fields Immunity in accordance With EN 61000-4-8 | Compliant |
| | Voltage Dips/Interruptions Immunity in accordance with EN 61000-4-11 | Compliant |
| | Broadband impulse noise disturbances, repetitive | N/A |
| Broadband impulse noise disturbances, isolated | N/A | |

N/A: not applicable




3. Conducted Emission

3.1 Measurement Uncertainty

Base on NIS 81, The Treatment of Uncertainty in EMC Measurements, the best estimate of the uncertainty of any conducted emissions measurement:

| Measurement uncertainty | | |
|-------------------------|------------|--------------------------------|
| Parameter | Conditions | Uncertainty |
| Conducted Emissions | Conducted | 9-150kHz $\pm 3.74\text{dB}$ |
| | | 0.15-30MHz $\pm 3.34\text{dB}$ |

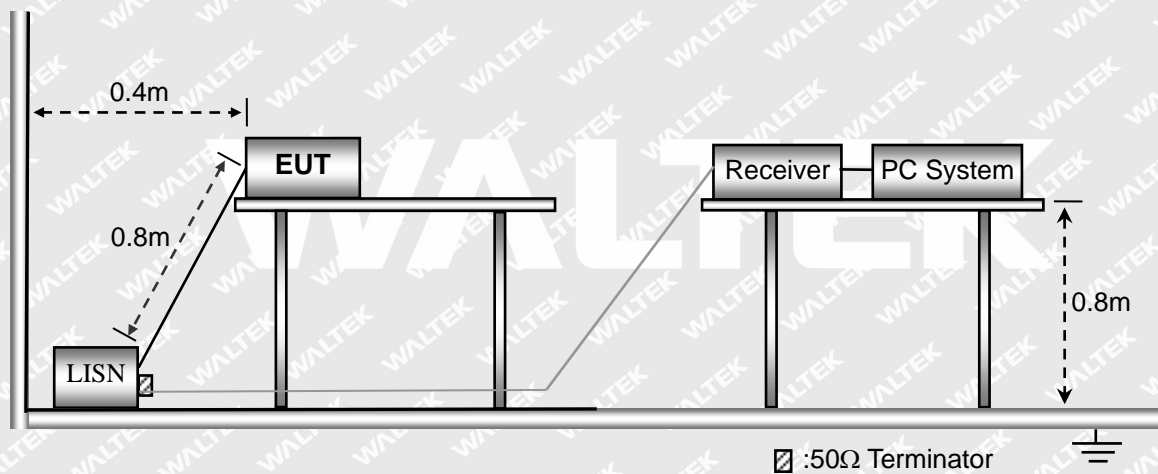3.2 Basic Test Setup Block Diagram





3.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 21.5 ° C |
| Relative Humidity: | 48 % |
| ATM Pressure: | 1012 mbar |

3.4 Summary of Test Results


Please find the results below:

WALTEK



GTM96180-1811-2.0-T3


| | | | |
|------------|-----|-----------|------|
| Test mode: | TM1 | Polarity: | Line |
|------------|-----|-----------|------|

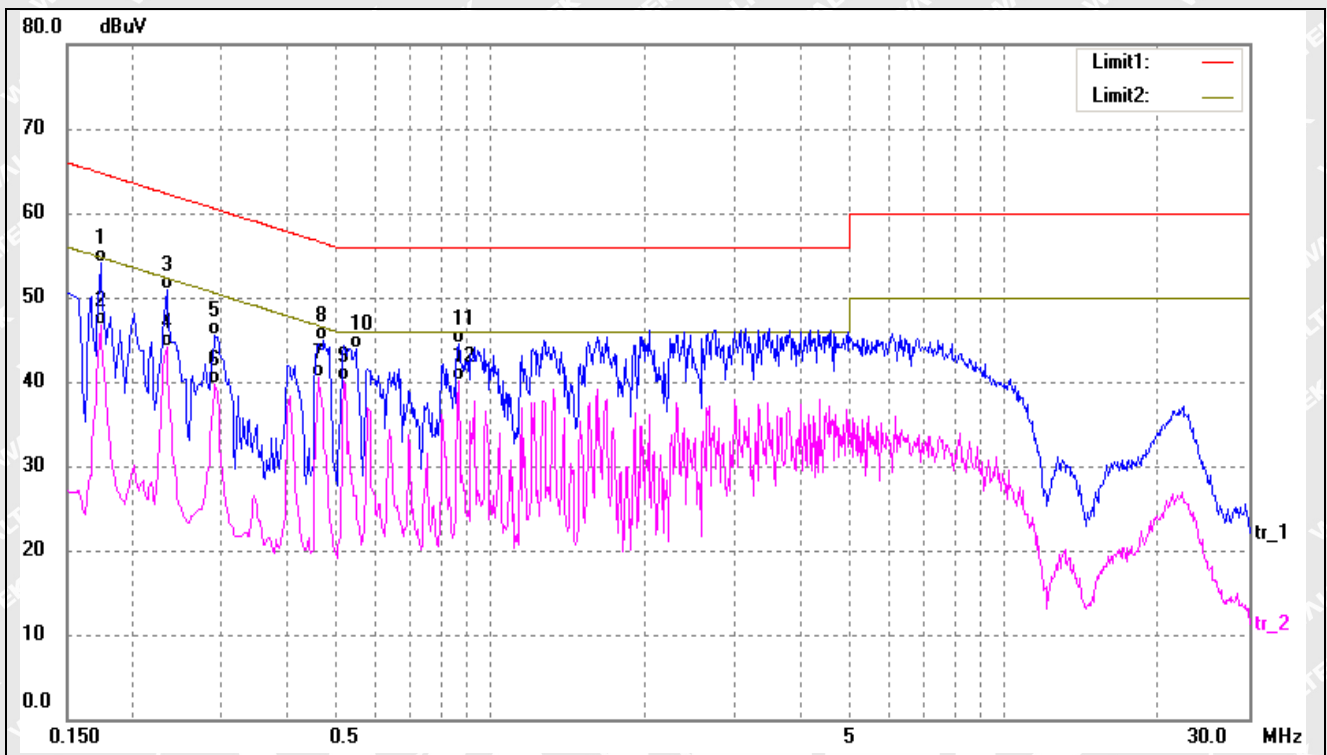

| No. | Frequency (MHz) | Reading (dBuV) | Correct (dB/m) | Result (dBuV) | Limit (dBuV) | Margin (dB) | Detector |
|-----|-----------------|----------------|----------------|---------------|--------------|-------------|----------|
| 1 | 0.1739 | 43.80 | 10.25 | 54.05 | 64.77 | -10.72 | QP |
| 2 | 0.1739 | 36.36 | 10.25 | 46.61 | 54.77 | -8.16 | AVG |
| 3 | 0.2340 | 40.68 | 10.26 | 50.94 | 62.30 | -11.36 | QP |
| 4 | 0.2340 | 33.88 | 10.26 | 44.14 | 52.30 | -8.16 | AVG |
| 5 | 0.2899 | 35.18 | 10.24 | 45.42 | 60.52 | -15.10 | QP |
| 6 | 0.2899 | 29.55 | 10.24 | 39.79 | 50.52 | -10.73 | AVG |
| 7 | 0.4620 | 30.32 | 10.22 | 40.54 | 46.66 | -6.12 | AVG |
| 8 | 0.4739 | 34.72 | 10.23 | 44.95 | 56.45 | -11.50 | QP |
| 9* | 0.5180 | 29.97 | 10.22 | 40.19 | 46.00 | -5.81 | AVG |
| 10 | 0.5460 | 33.74 | 10.21 | 43.95 | 56.00 | -12.05 | QP |
| 11 | 0.8699 | 34.27 | 10.21 | 44.48 | 56.00 | -11.52 | QP |
| 12 | 0.8699 | 29.83 | 10.21 | 40.04 | 46.00 | -5.96 | AVG |



| | | | |
|------------|-----|-----------|---------|
| Test mode: | TM1 | Polarity: | Neutral |
|------------|-----|-----------|---------|

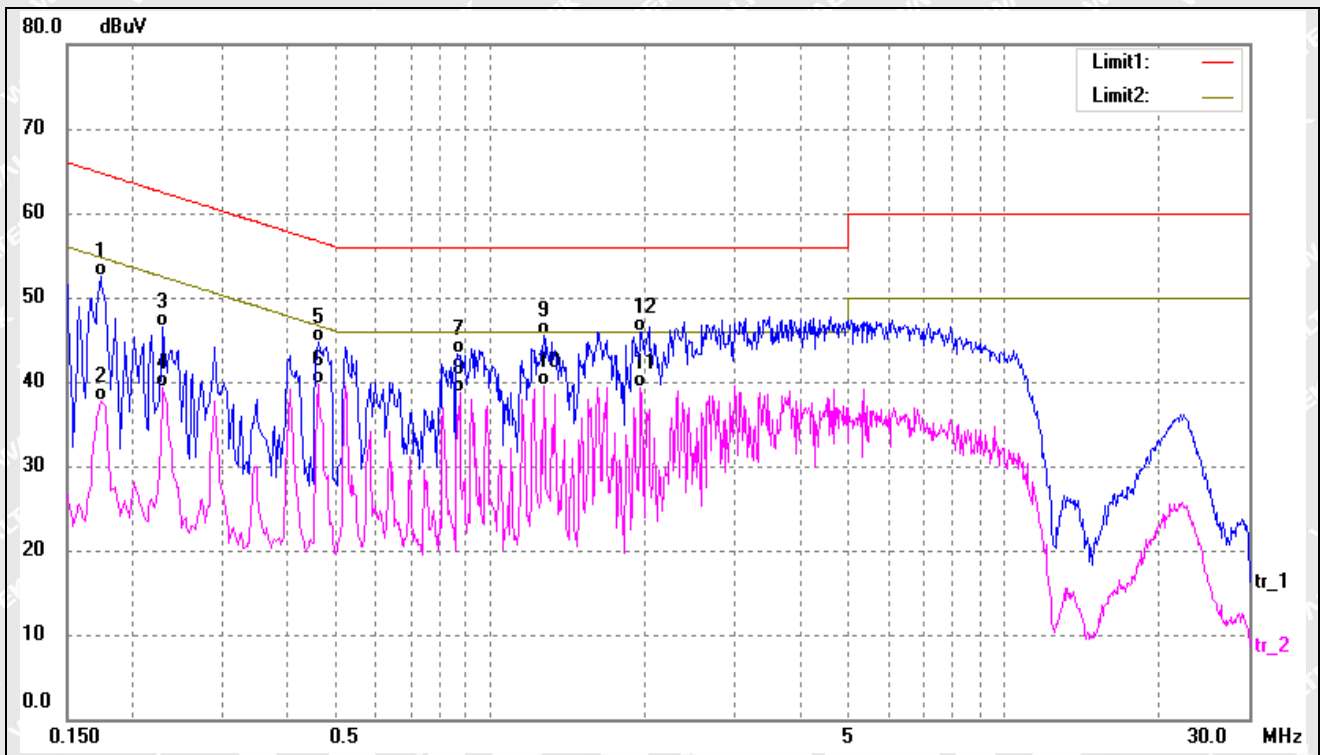


| No. | Frequency (MHz) | Reading (dBuV) | Correct (dB/m) | Result (dBuV) | Limit (dBuV) | Margin (dB) | Detector |
|-----|-----------------|----------------|----------------|---------------|--------------|-------------|----------|
| 1 | 0.1737 | 42.31 | 10.26 | 52.57 | 64.78 | -12.21 | QP |
| 2 | 0.1737 | 27.41 | 10.26 | 37.67 | 54.78 | -17.11 | AVG |
| 3 | 0.2300 | 36.19 | 10.26 | 46.45 | 62.45 | -16.00 | QP |
| 4 | 0.2300 | 29.00 | 10.26 | 39.26 | 52.45 | -13.19 | AVG |
| 5 | 0.4620 | 34.44 | 10.22 | 44.66 | 56.66 | -12.00 | QP |
| 6 | 0.4620 | 29.55 | 10.22 | 39.77 | 46.66 | -6.89 | AVG |
| 7 | 0.8659 | 33.05 | 10.21 | 43.26 | 56.00 | -12.74 | QP |
| 8 | 0.8739 | 28.49 | 10.21 | 38.70 | 46.00 | -7.30 | AVG |
| 9 | 1.2700 | 35.34 | 10.21 | 45.55 | 56.00 | -10.45 | QP |
| 10* | 1.2700 | 29.24 | 10.21 | 39.45 | 46.00 | -6.55 | AVG |
| 11 | 1.9618 | 29.07 | 10.28 | 39.35 | 46.00 | -6.65 | AVG |
| 12 | 1.9738 | 35.62 | 10.29 | 45.91 | 56.00 | -10.09 | QP |



GTM91120-3024-T3A


| | | | |
|------------|-----|-----------|------|
| Test mode: | TM2 | Polarity: | Line |
|------------|-----|-----------|------|

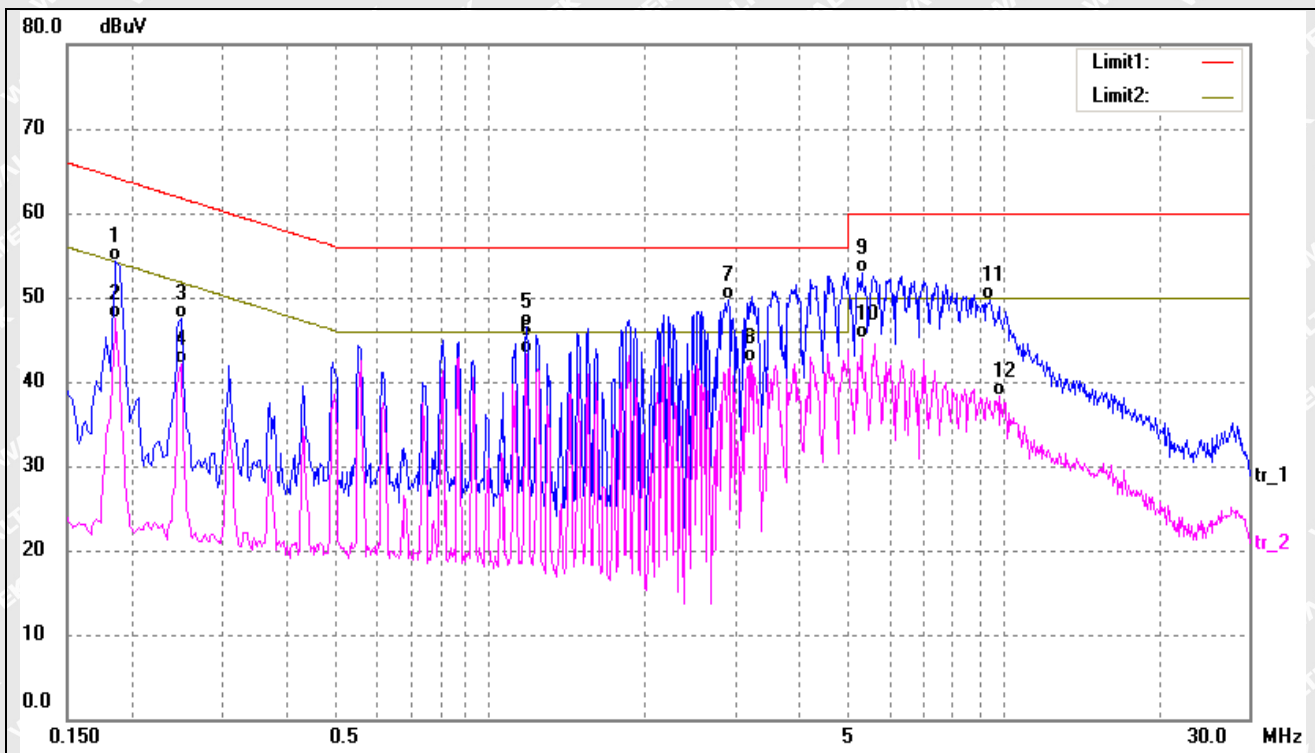

| No. | Frequency (MHz) | Reading (dBuV) | Correct (dB/m) | Result (dBuV) | Limit (dBuV) | Margin (dB) | Detector |
|-----|-----------------|----------------|----------------|---------------|--------------|-------------|----------|
| 1 | 0.1860 | 43.97 | 10.26 | 54.23 | 64.21 | -9.98 | QP |
| 2 | 0.1860 | 37.30 | 10.26 | 47.56 | 54.21 | -6.65 | AVG |
| 3 | 0.2500 | 37.18 | 10.26 | 47.44 | 61.75 | -14.31 | QP |
| 4 | 0.2500 | 31.92 | 10.26 | 42.18 | 51.75 | -9.57 | AVG |
| 5 | 1.1780 | 36.26 | 10.22 | 46.48 | 56.00 | -9.52 | QP |
| 6* | 1.1780 | 33.15 | 10.22 | 43.37 | 46.00 | -2.63 | AVG |
| 7 | 2.9020 | 39.43 | 10.27 | 49.70 | 56.00 | -6.30 | QP |
| 8 | 3.2100 | 31.96 | 10.27 | 42.23 | 46.00 | -3.77 | AVG |
| 9 | 5.3020 | 42.77 | 10.22 | 52.99 | 60.00 | -7.01 | QP |
| 10 | 5.3020 | 34.84 | 10.22 | 45.06 | 50.00 | -4.94 | AVG |
| 11 | 9.4340 | 39.45 | 10.28 | 49.73 | 60.00 | -10.27 | QP |
| 12 | 9.7980 | 27.99 | 10.28 | 38.27 | 50.00 | -11.73 | AVG |



| | | | |
|------------|-----|-----------|---------|
| Test mode: | TM2 | Polarity: | Neutral |
|------------|-----|-----------|---------|

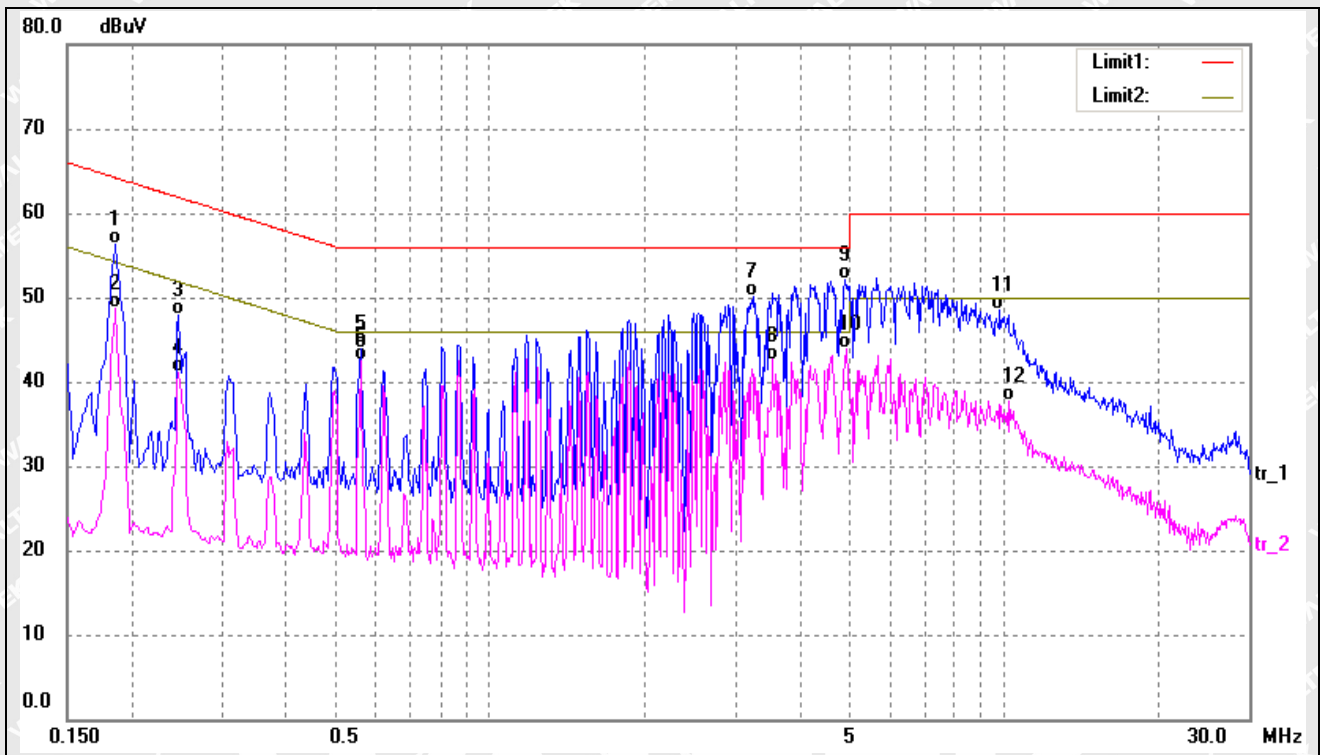


| No. | Frequency (MHz) | Reading (dBuV) | Correct (dB/m) | Result (dBuV) | Limit (dBuV) | Margin (dB) | Detector |
|-----|-----------------|----------------|----------------|---------------|--------------|-------------|----------|
| 1 | 0.1860 | 46.09 | 10.26 | 56.35 | 64.21 | -7.86 | QP |
| 2 | 0.1860 | 38.50 | 10.26 | 48.76 | 54.21 | -5.45 | AVG |
| 3 | 0.2460 | 37.65 | 10.26 | 47.91 | 61.89 | -13.98 | QP |
| 4 | 0.2460 | 30.77 | 10.26 | 41.03 | 51.89 | -10.86 | AVG |
| 5 | 0.5580 | 33.61 | 10.21 | 43.82 | 56.00 | -12.18 | QP |
| 6 | 0.5580 | 32.28 | 10.21 | 42.49 | 46.00 | -3.51 | AVG |
| 7 | 3.2700 | 39.81 | 10.26 | 50.07 | 56.00 | -5.93 | QP |
| 8 | 3.5540 | 32.34 | 10.26 | 42.60 | 46.00 | -3.40 | AVG |
| 9 | 4.9140 | 41.88 | 10.22 | 52.10 | 56.00 | -3.90 | QP |
| 10* | 4.9380 | 33.62 | 10.22 | 43.84 | 46.00 | -2.16 | AVG |
| 11 | 9.8300 | 38.26 | 10.28 | 48.54 | 60.00 | -11.46 | QP |
| 12 | 10.1820 | 27.43 | 10.29 | 37.72 | 50.00 | -12.28 | AVG |



GTM96300-3624-T2


| | | | |
|------------|-----|-----------|------|
| Test mode: | TM3 | Polarity: | Line |
|------------|-----|-----------|------|

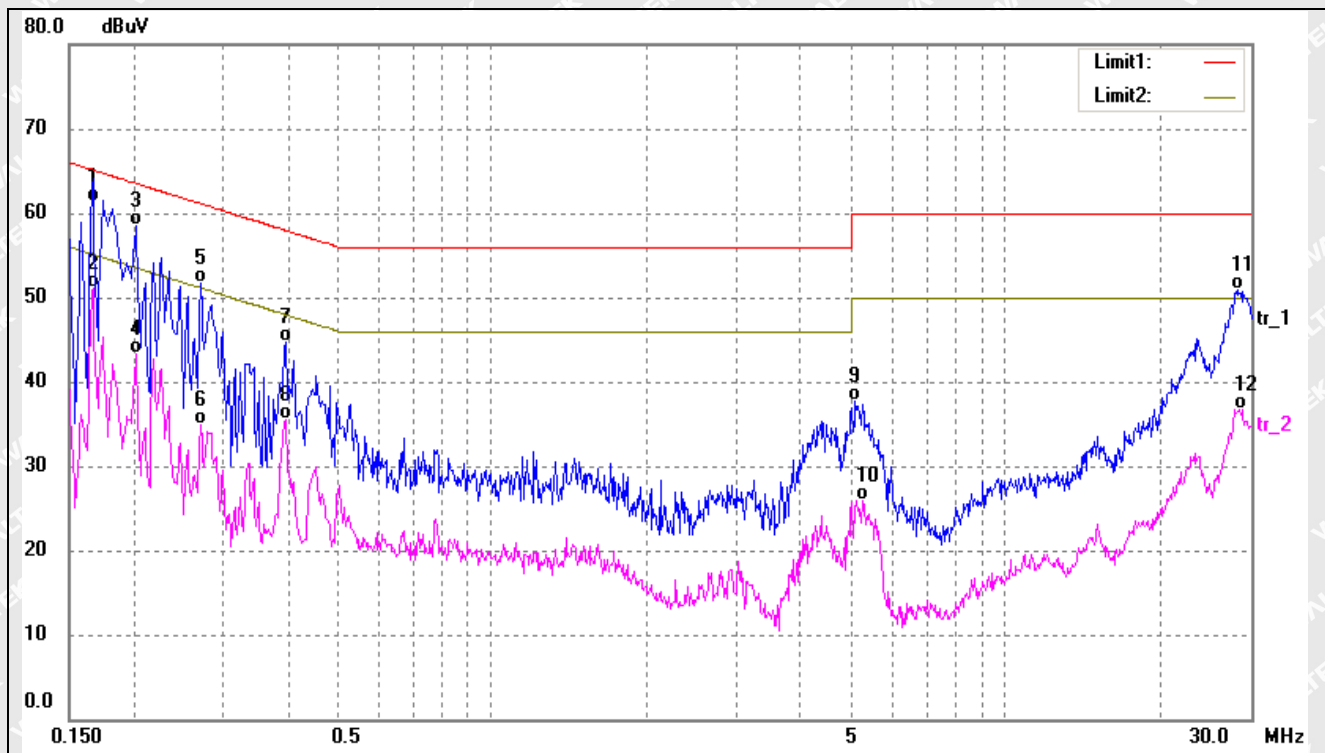

| No. | Frequency (MHz) | Reading (dBuV) | Correct (dB/m) | Result (dBuV) | Limit (dBuV) | Margin (dB) | Detector |
|-----|-----------------|----------------|----------------|---------------|--------------|-------------|----------|
| 1* | 0.1660 | 51.03 | 10.26 | 61.29 | 65.15 | -3.86 | QP |
| 2 | 0.1660 | 40.85 | 10.26 | 51.11 | 55.15 | -4.04 | AVG |
| 3 | 0.2020 | 48.15 | 10.27 | 58.42 | 63.52 | -5.10 | QP |
| 4 | 0.2020 | 32.97 | 10.27 | 43.24 | 53.52 | -10.28 | AVG |
| 5 | 0.2700 | 41.40 | 10.25 | 51.65 | 61.12 | -9.47 | QP |
| 6 | 0.2700 | 24.57 | 10.25 | 34.82 | 51.12 | -16.30 | AVG |
| 7 | 0.3940 | 34.42 | 10.23 | 44.65 | 57.98 | -13.33 | QP |
| 8 | 0.3940 | 25.29 | 10.23 | 35.52 | 47.98 | -12.46 | AVG |
| 9 | 5.0980 | 27.54 | 10.22 | 37.76 | 60.00 | -22.24 | QP |
| 10 | 5.2500 | 15.76 | 10.22 | 25.98 | 50.00 | -24.02 | AVG |
| 11 | 28.4380 | 40.22 | 10.69 | 50.91 | 60.00 | -9.09 | QP |
| 12 | 28.8020 | 26.06 | 10.70 | 36.76 | 50.00 | -13.24 | AVG |



| | | | |
|------------|-----|-----------|---------|
| Test mode: | TM3 | Polarity: | Neutral |
|------------|-----|-----------|---------|

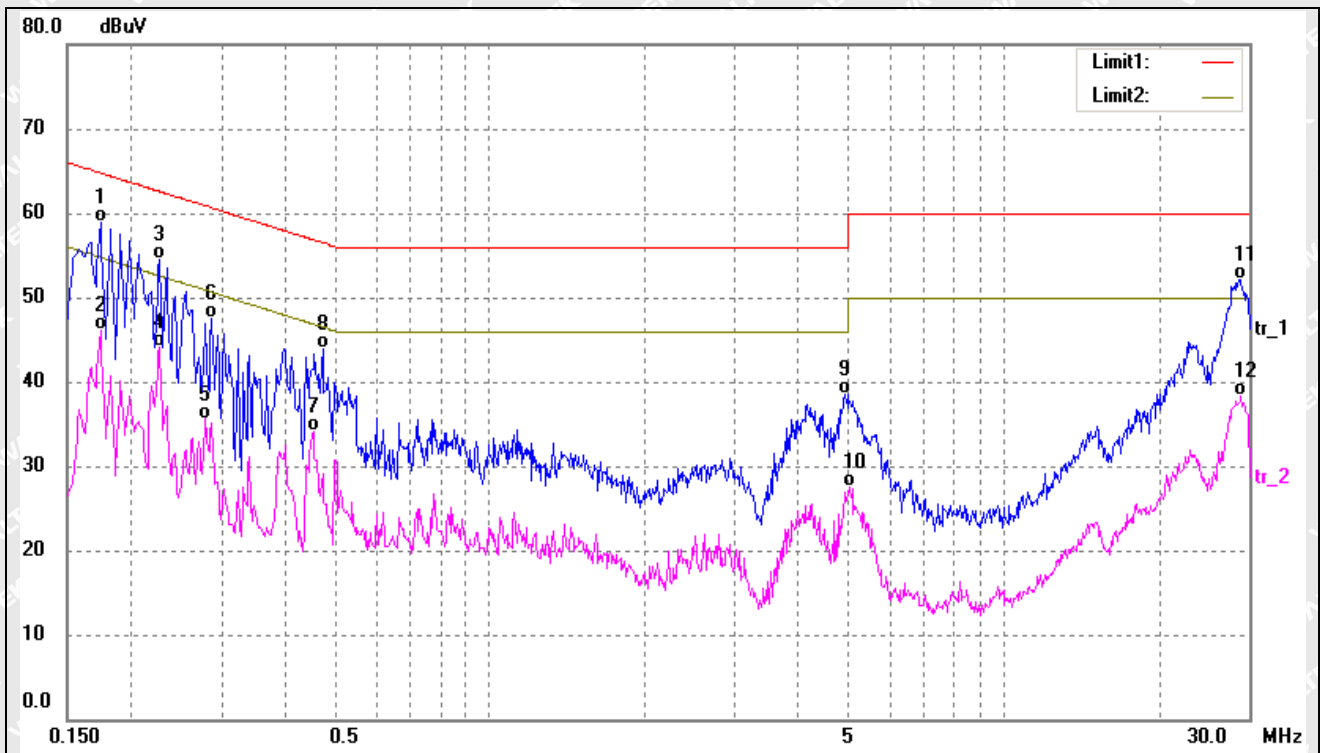

| No. | Frequency (MHz) | Reading (dBuV) | Correct (dB/m) | Result (dBuV) | Limit (dBuV) | Margin (dB) | Detector |
|-----|--------------------|-------------------|-------------------|------------------|-----------------|----------------|----------|
| 1* | 0.1740 | 48.75 | 10.25 | 59.00 | 64.76 | -5.76 | QP |
| 2 | 0.1740 | 35.85 | 10.25 | 46.10 | 54.76 | -8.66 | AVG |
| 3 | 0.2260 | 44.30 | 10.26 | 54.56 | 62.59 | -8.03 | QP |
| 4 | 0.2260 | 33.91 | 10.26 | 44.17 | 52.59 | -8.42 | AVG |
| 5 | 0.2779 | 25.35 | 10.25 | 35.60 | 50.88 | -15.28 | AVG |
| 6 | 0.2860 | 37.25 | 10.25 | 47.50 | 60.64 | -13.14 | QP |
| 7 | 0.4500 | 23.93 | 10.22 | 34.15 | 46.87 | -12.72 | AVG |
| 8 | 0.4700 | 33.74 | 10.23 | 43.97 | 56.51 | -12.54 | QP |
| 9 | 4.9140 | 28.34 | 10.22 | 38.56 | 56.00 | -17.44 | QP |
| 10 | 5.0260 | 17.19 | 10.22 | 27.41 | 50.00 | -22.59 | AVG |
| 11 | 28.6580 | 41.41 | 10.69 | 52.10 | 60.00 | -7.90 | QP |
| 12 | 29.0020 | 27.61 | 10.70 | 38.31 | 50.00 | -11.69 | AVG |




4. Radiated Emission

4.1 Measurement Uncertainty

Base on NIS 81, The Treatment of Uncertainty in EMC Measurements, the best estimate of the uncertainty of any radiation emissions measurement:

| Measurement uncertainty | | |
|-------------------------|------------|-------------------------------|
| Parameter | Conditions | Uncertainty |
| Radiated Emissions | Radiated | 30-200MHz $\pm 4.52\text{dB}$ |
| | | 0.2-1GHz $\pm 5.56\text{dB}$ |
| | | 1-6GHz $\pm 3.84\text{dB}$ |
| | | 6-18GHz $\pm 3.92\text{dB}$ |

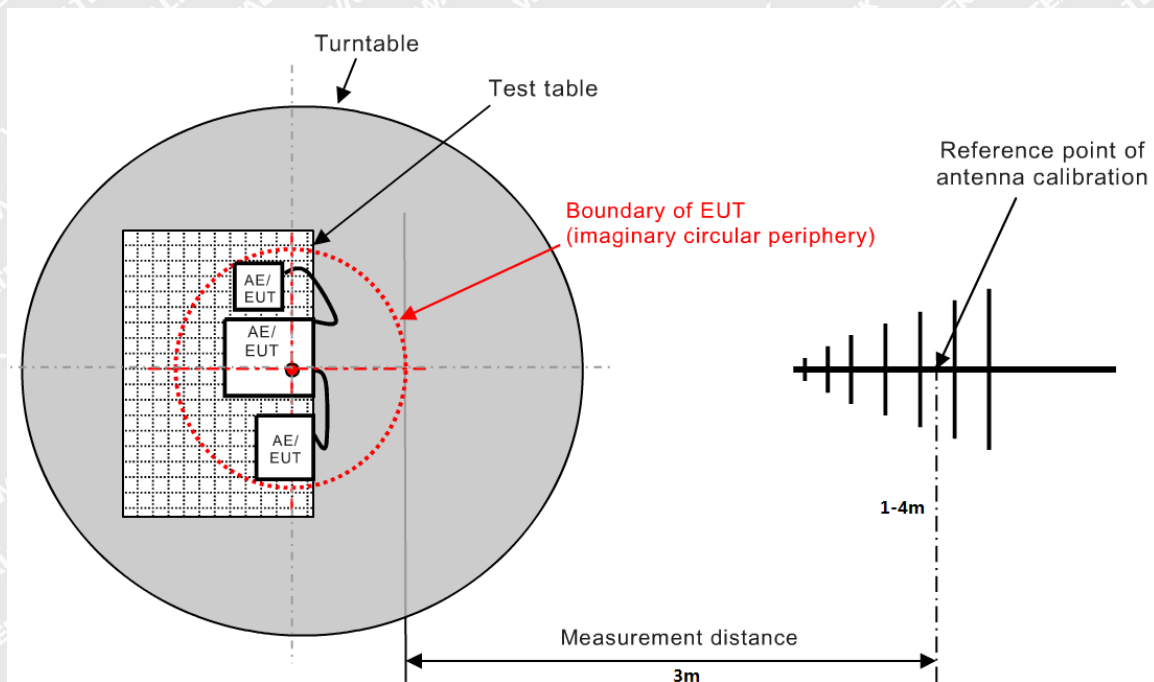4.2 Basic Test Setup Block Diagram





4.3 Corrected Amplitude & Margin Calculation

The Corrected Amplitude is calculated by adding the Antenna Factor and the Cable Factor, and subtracting the Amplifier Gain from the Amplitude reading. The basic equation is as follows:

$$\text{Corr. Ampl.} = \text{Indicated Reading} + \text{Correct Correct} = \text{Ant.Factor} + \text{Cable Loss} - \text{Ampl.Gain}$$

The “**Margin**” column of the following data tables indicates the degree of compliance with the applicable limit. For example, a margin of -6dB μ V means the emission is 6dB μ V below the maximum limit for Class B device. The equation for margin calculation is as follows:

$$\text{Margin} = \text{Corr. Ampl.} - \text{EN 55032 Class B Limit}$$

4.4 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 23.5° C |
| Relative Humidity: | 54 % |
| ATM Pressure: | 1010 mbar |


4.5 Summary of Test Results

Please find the results below:



GTM96180-1811-2.0-T3


| | | | |
|------------|-----|-----------|------------|
| Test mode: | TM1 | Polarity: | Horizontal |
|------------|-----|-----------|------------|

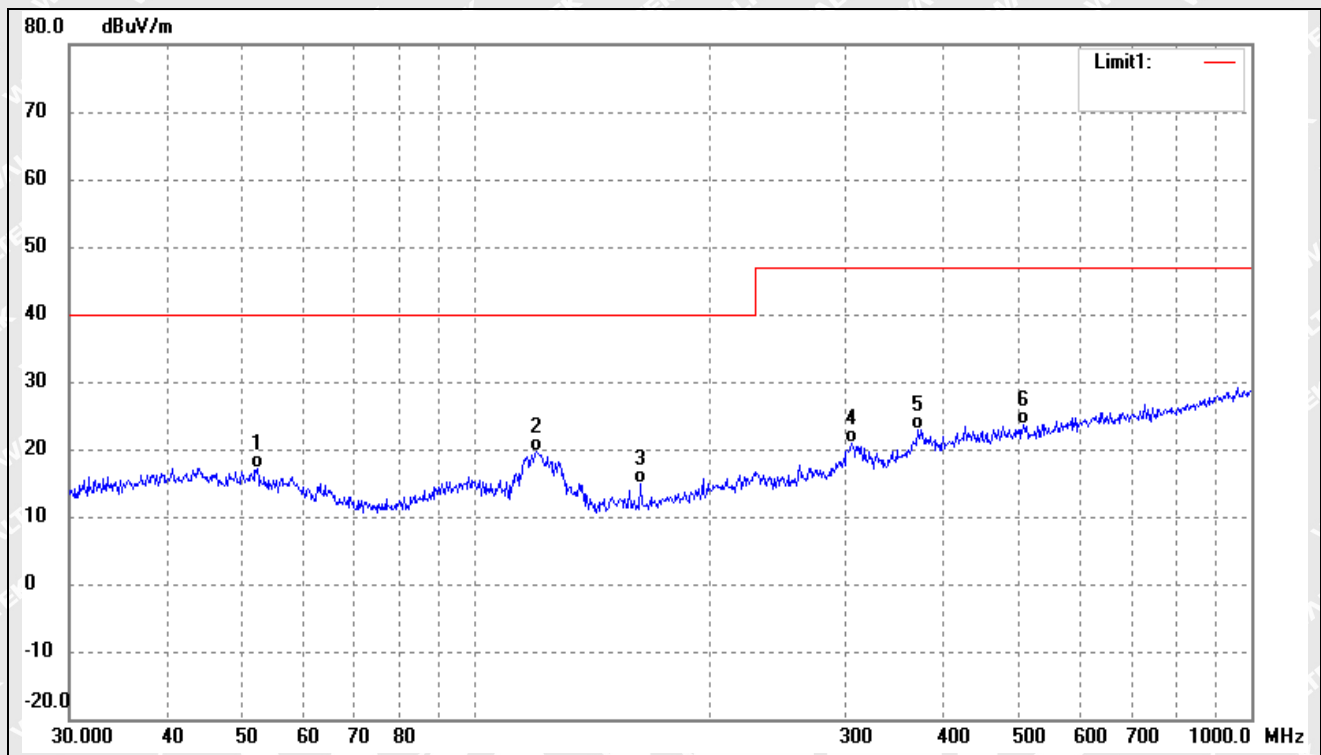

| No. | Frequency (MHz) | Reading (dBuV/m) | Correct dB/m | Result (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Degree (°) | Height (cm) | Remark |
|-----|--------------------|---------------------|-----------------|--------------------|-------------------|----------------|---------------|----------------|--------|
| 1 | 52.3912 | 28.52 | -11.34 | 17.18 | 40.00 | -22.82 | 281 | 100 | QP |
| 2 | 119.8555 | 33.52 | -13.91 | 19.61 | 40.00 | -20.39 | 92 | 100 | QP |
| 3 | 163.1818 | 29.45 | -14.68 | 14.77 | 40.00 | -25.23 | 331 | 100 | QP |
| 4 | 305.6800 | 29.95 | -9.17 | 20.78 | 47.00 | -26.22 | 97 | 100 | QP |
| 5 | 372.0045 | 30.05 | -7.08 | 22.97 | 47.00 | -24.03 | 217 | 100 | QP |
| 6 | 508.2581 | 28.70 | -5.09 | 23.61 | 47.00 | -23.39 | 115 | 100 | QP |



| | | | |
|------------|-----|-----------|----------|
| Test mode: | TM1 | Polarity: | Vertical |
|------------|-----|-----------|----------|

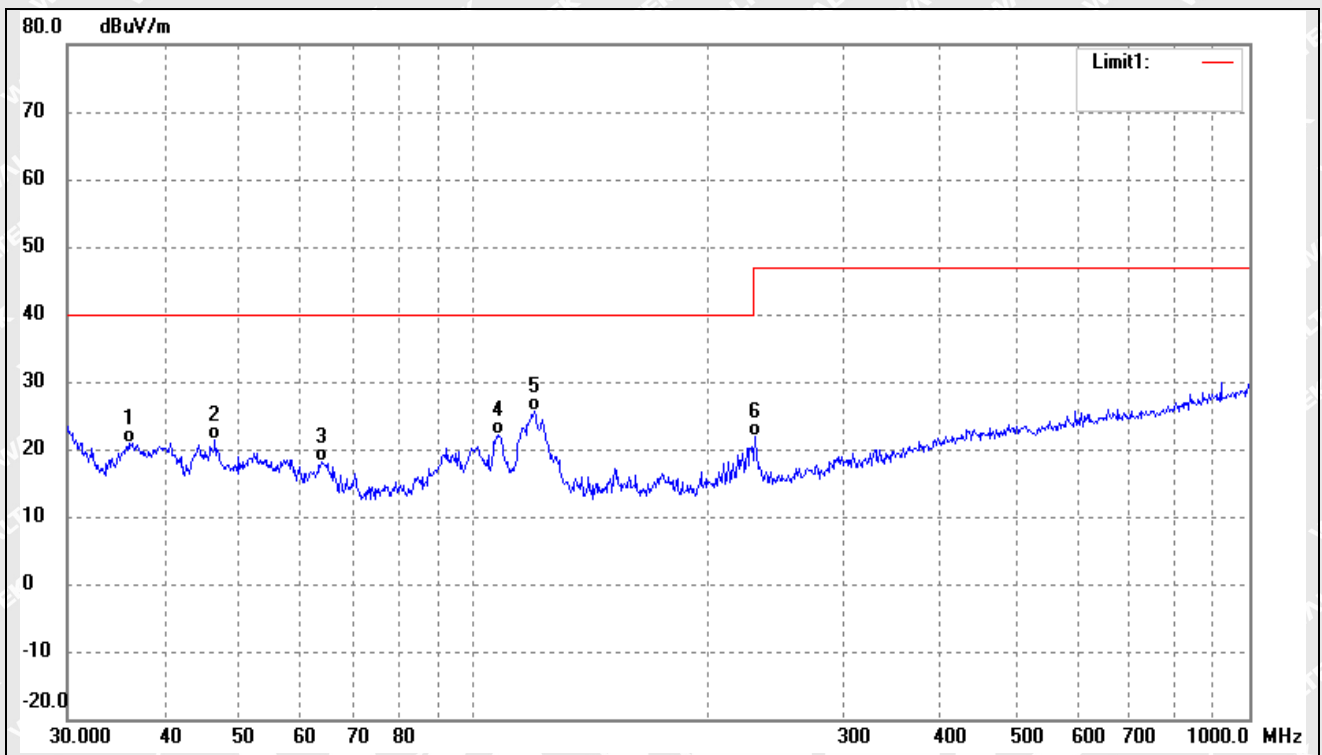


| No. | Frequency (MHz) | Reading (dBuV/m) | Correct (dB/m) | Result (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Degree (°) | Height (cm) | Remark |
|-----|-----------------|------------------|----------------|-----------------|----------------|-------------|------------|-------------|--------|
| 1 | 36.0007 | 32.57 | -11.61 | 20.96 | 40.00 | -19.04 | 149 | 100 | QP |
| 2 | 46.5030 | 32.24 | -10.89 | 21.35 | 40.00 | -18.65 | 114 | 100 | QP |
| 3 | 63.7588 | 31.90 | -13.68 | 18.22 | 40.00 | -21.78 | 97 | 100 | QP |
| 4 | 107.5101 | 34.70 | -12.47 | 22.23 | 40.00 | -17.77 | 132 | 100 | QP |
| 5 | 119.8556 | 39.48 | -13.91 | 25.57 | 40.00 | -14.43 | 184 | 100 | QP |
| 6 | 230.9068 | 33.42 | -11.49 | 21.93 | 47.00 | -25.07 | 308 | 100 | QP |



GTM91120-3024-T3A


| | | | |
|------------|-----|-----------|------------|
| Test mode: | TM2 | Polarity: | Horizontal |
|------------|-----|-----------|------------|

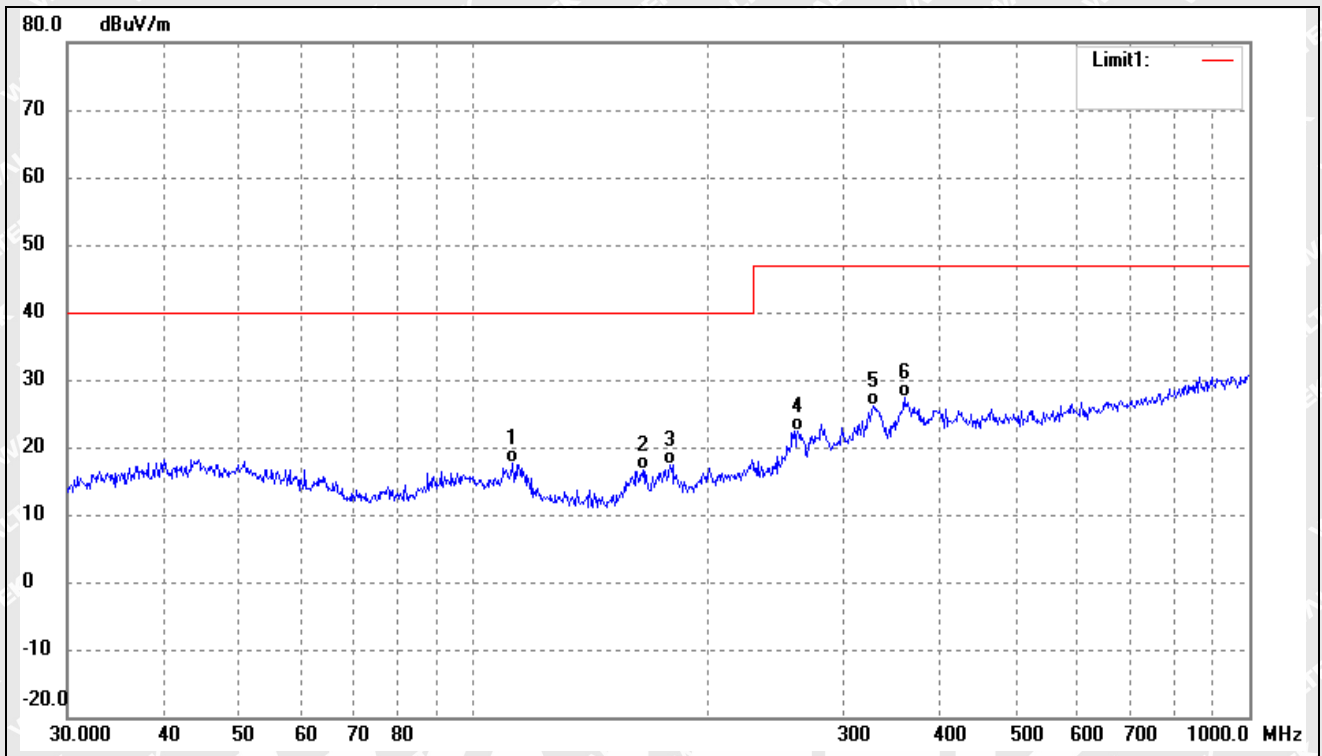

| No. | Frequency (MHz) | Reading (dBuV/m) | Correct (dB/m) | Result (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Degree (°) | Height (cm) | Remark |
|-----|-----------------|------------------|----------------|-----------------|----------------|-------------|------------|-------------|--------|
| 1 | 112.5244 | 29.86 | -12.28 | 17.58 | 40.00 | -22.42 | 54 | 100 | QP |
| 2 | 165.4866 | 30.41 | -13.67 | 16.74 | 40.00 | -23.26 | 160 | 100 | QP |
| 3 | 179.3863 | 30.47 | -13.05 | 17.42 | 40.00 | -22.58 | 90 | 100 | QP |
| 4 | 261.9753 | 31.46 | -9.05 | 22.41 | 47.00 | -24.59 | 345 | 100 | QP |
| 5 | 327.8873 | 32.86 | -6.83 | 26.03 | 47.00 | -20.97 | 275 | 100 | QP |
| 6 | 359.1860 | 33.17 | -5.79 | 27.38 | 47.00 | -19.62 | 303 | 100 | QP |



| | | | |
|------------|-----|-----------|----------|
| Test mode: | TM2 | Polarity: | Vertical |
|------------|-----|-----------|----------|

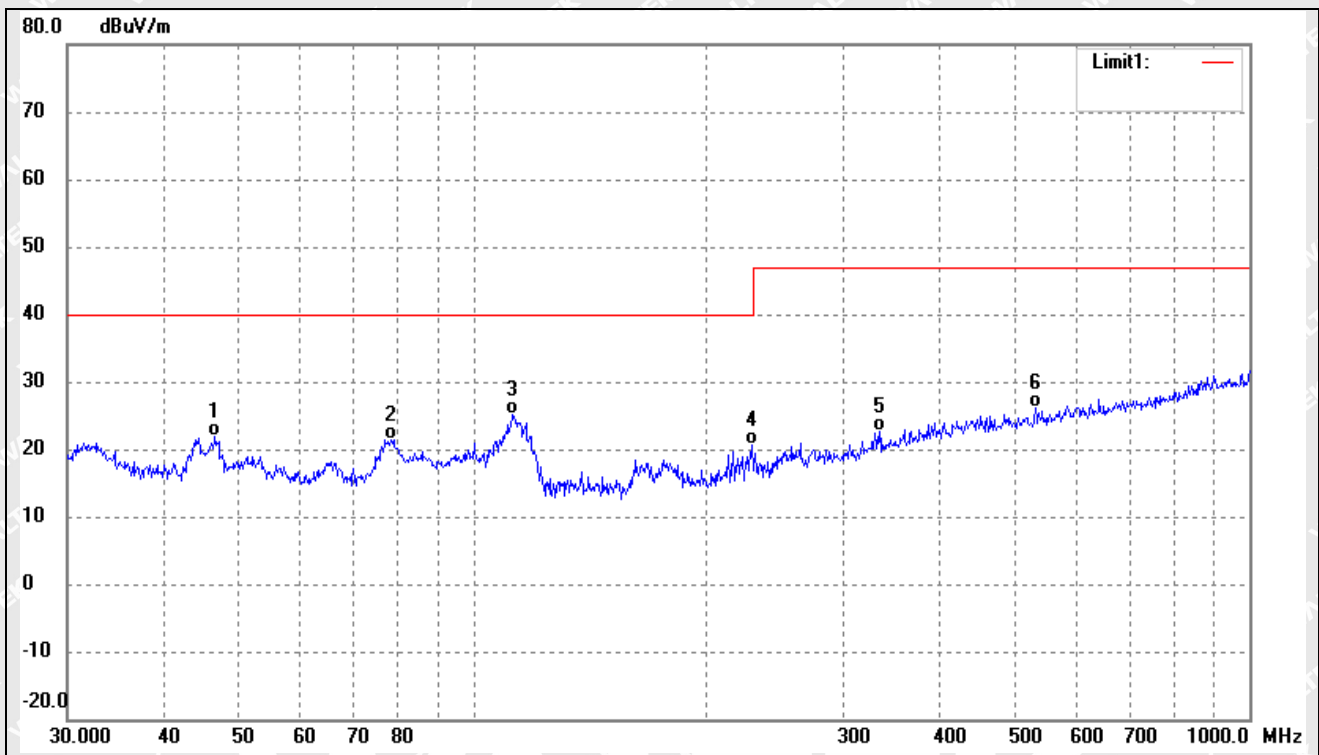


| No. | Frequency (MHz) | Reading (dBuV/m) | Correct dB/m | Result (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Degree (°) | Height (cm) | Remark |
|-----|--------------------|---------------------|-----------------|--------------------|-------------------|----------------|---------------|----------------|--------|
| 1 | 46.5030 | 31.81 | -9.91 | 21.90 | 40.00 | -18.10 | 269 | 100 | QP |
| 2 | 78.4133 | 35.49 | -14.06 | 21.43 | 40.00 | -18.57 | 161 | 100 | QP |
| 3 | 112.5244 | 37.37 | -12.28 | 25.09 | 40.00 | -14.91 | 67 | 100 | QP |
| 4 | 228.4904 | 30.86 | -10.28 | 20.58 | 40.00 | -19.42 | 311 | 100 | QP |
| 5 | 333.6867 | 29.27 | -6.67 | 22.60 | 47.00 | -24.40 | 140 | 100 | QP |
| 6 | 530.1014 | 29.52 | -3.29 | 26.23 | 47.00 | -20.77 | 230 | 100 | QP |



GTM96300-3624-T2


| | | | |
|------------|-----|-----------|------------|
| Test mode: | TM3 | Polarity: | Horizontal |
|------------|-----|-----------|------------|

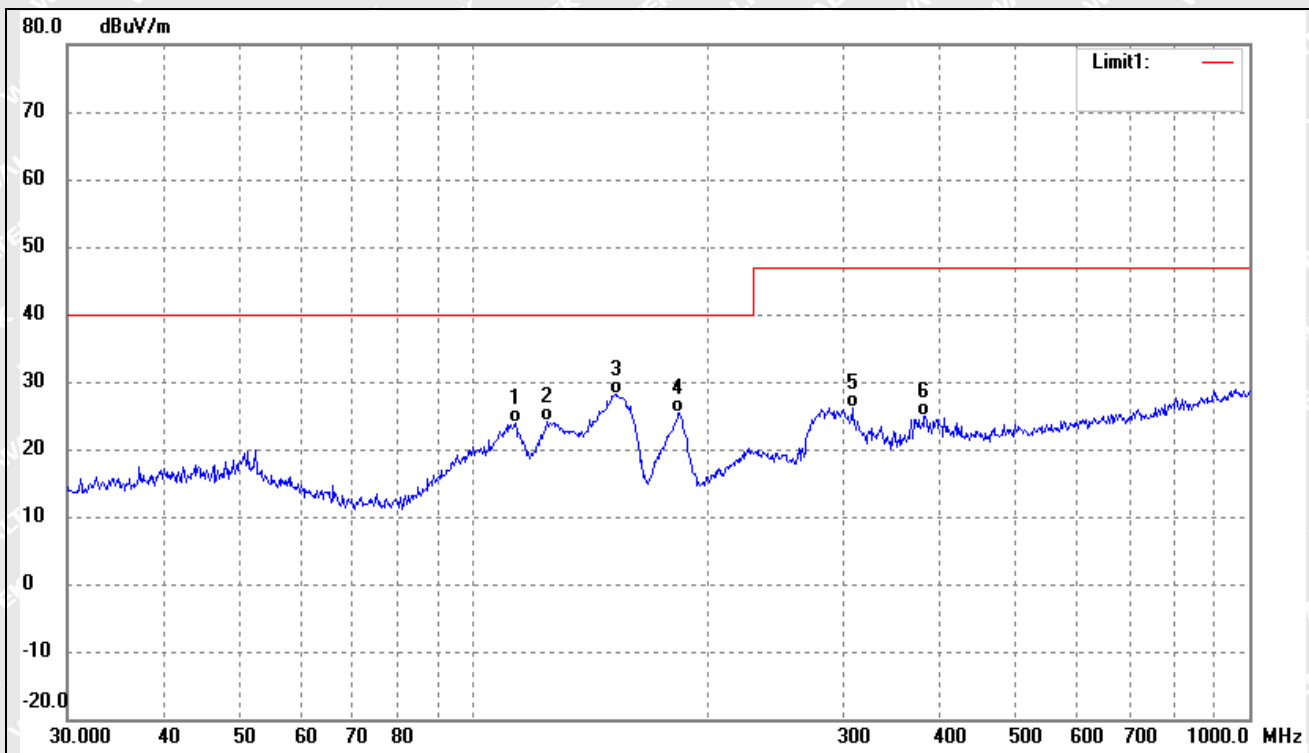

| No. | Frequency (MHz) | Reading (dBuV/m) | Correct (dB/m) | Result (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Degree (°) | Height (cm) | Remark |
|-----|-----------------|------------------|----------------|-----------------|----------------|-------------|------------|-------------|--------|
| 1 | 113.3163 | 36.92 | -13.04 | 23.88 | 40.00 | -16.12 | 115 | 100 | QP |
| 2 | 124.5690 | 38.54 | -14.33 | 24.21 | 40.00 | -15.79 | 177 | 100 | QP |
| 3 | 152.6641 | 43.39 | -15.16 | 28.23 | 40.00 | -11.77 | 117 | 100 | QP |
| 4 | 183.8440 | 38.95 | -13.55 | 25.40 | 40.00 | -14.60 | 98 | 100 | QP |
| 5 | 307.8313 | 35.33 | -9.11 | 26.22 | 47.00 | -20.78 | 321 | 100 | QP |
| 6 | 381.2487 | 31.60 | -6.75 | 24.85 | 47.00 | -22.15 | 343 | 100 | QP |



| | | | |
|------------|-----|-----------|----------|
| Test mode: | TM3 | Polarity: | Vertical |
|------------|-----|-----------|----------|

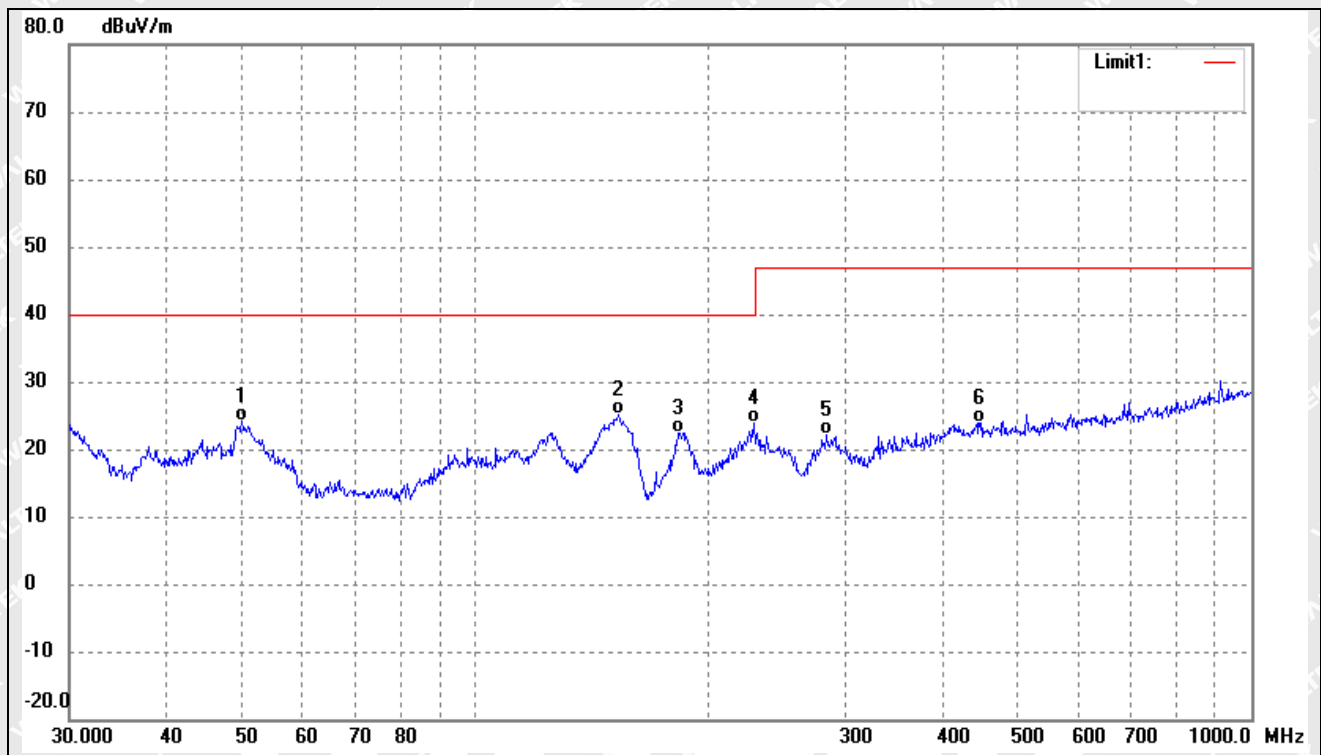

| No. | Frequency (MHz) | Reading (dBuV/m) | Correct dB/m | Result (dBuV/m) | Limit (dBuV/m) | Margin (dB) | Degree (°) | Height (cm) | Remark |
|-----|--------------------|---------------------|-----------------|--------------------|-------------------|----------------|---------------|----------------|--------|
| 1 | 50.0566 | 35.05 | -10.90 | 24.15 | 40.00 | -15.85 | 69 | 100 | QP |
| 2 | 153.2004 | 40.28 | -15.14 | 25.14 | 40.00 | -14.86 | 98 | 100 | QP |
| 3 | 182.5592 | 36.18 | -13.71 | 22.47 | 40.00 | -17.53 | 81 | 100 | QP |
| 4 | 228.4904 | 35.50 | -11.55 | 23.95 | 40.00 | -16.05 | 145 | 100 | QP |
| 5 | 283.9791 | 32.02 | -9.83 | 22.19 | 47.00 | -24.81 | 186 | 100 | QP |
| 6 | 446.4141 | 29.34 | -5.40 | 23.94 | 47.00 | -23.06 | 255 | 100 | QP |



5. Harmonic Current Emissions

5.1 Test Procedure

Test is conducted under the description of EN IEC 61000-3-2.


5.2 Test Standards

EN IEC 61000-3-2, Clause 7.1 Limits for Class A equipment.

5.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 23.5 °C |
| Relative Humidity: | 52 % |
| ATM Pressure: | 1013 mbar |

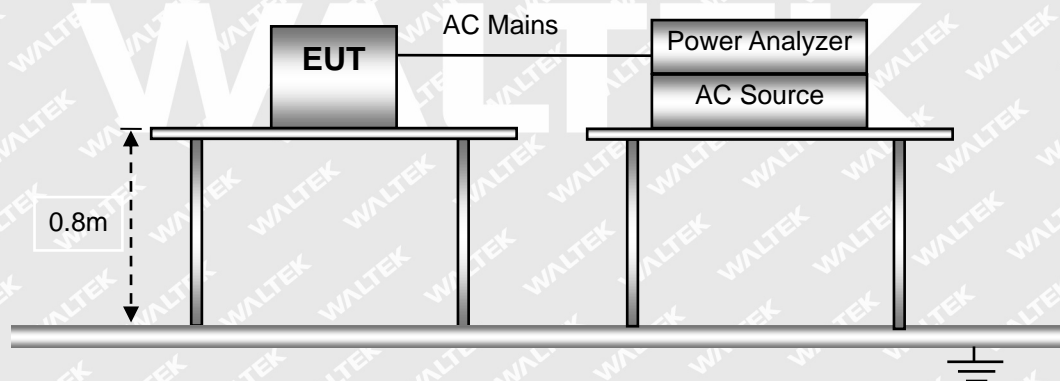5.4 Basic Test Setup Block Diagram



5.5 Harmonic Current Emissions Test Data

According to Clause 7 of EN IEC 61000-3-2, the rated power of the EUT is less than 75W, belong to 'equipment with a rated power of 75W or less', therefore 'limits are not specified in this edition of the standards'. It is deem to full fit the requirements of the standards.

Result: The EUT is compliance with the requirements of this section.



6. Voltage Fluctuation Flicker

6.1 Test Procedure

Test is conducted under the description of EN 61000-3-3.


6.2 Test Standards

EN 61000-3-3, Limit: Clause 5.

6.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 23.5 °C |
| Relative Humidity: | 52 % |
| ATM Pressure: | 1013 mbar |

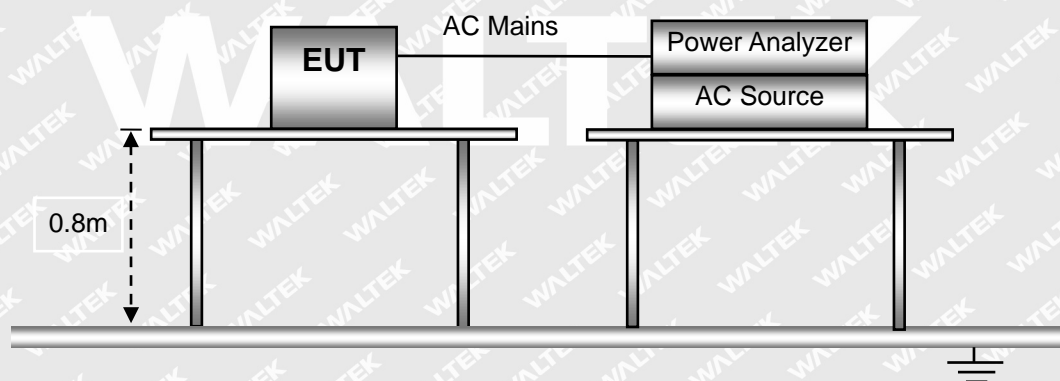6.4 Basic Test Setup Block Diagram



6.5 Voltage Fluctuation and Flicker Test Data



GTM96180-1811-2.0-T3

| | |
|------------|-----|
| Test mode: | TM1 |
|------------|-----|

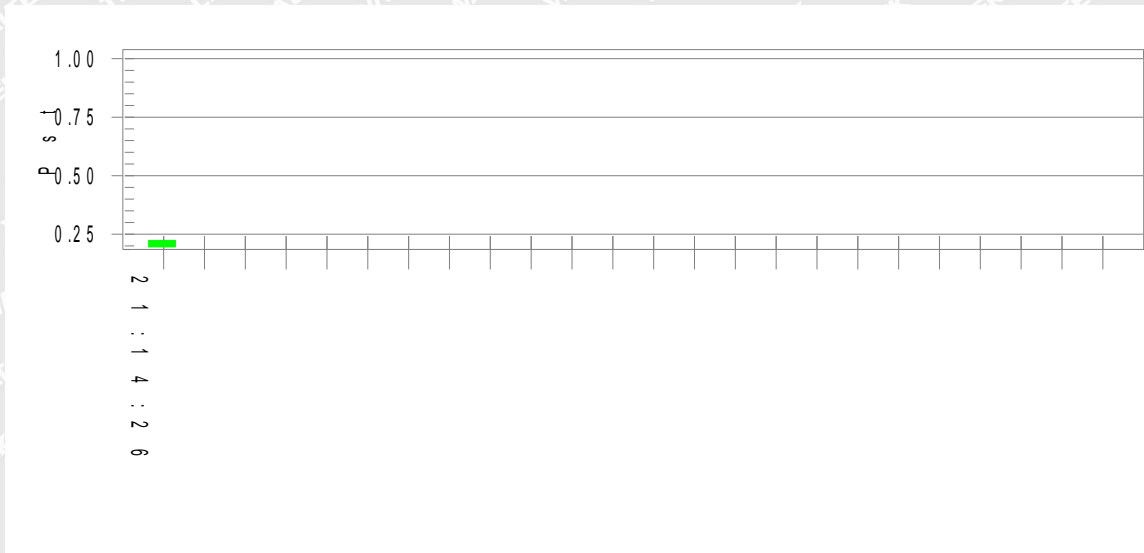
Flicker Test Summary per IEC61000-3-3:2013/AMD1:2017 (Run time)

Test Result: Pass

Status: Test Completed

Pst and limit line

European Limits



Plt and limit line



Parameter values recorded during the test:

Vrms at the end of test (Volt): 231.47

Highest dt (%):

T-max (mS): 0

Highest dc (%): 0.00

Highest dmax (%): 0.00

Highest Pst (10 min. period): 0.224

Highest Plt (2 hr. period): 0.098

Test limit (%):

Test limit (mS): 500.0 Pass

Test limit (%): 3.30 Pass

Test limit (%): 4.00 Pass

Test limit: 1.000 Pass

Test limit: 0.650 Pass

Waltek Testing Group (Shenzhen) Co., Ltd.

[Http://www.waltek.com.cn](http://www.waltek.com.cn)



GTM91120-3024-T3A

| | |
|------------|-----|
| Test mode: | TM2 |
|------------|-----|

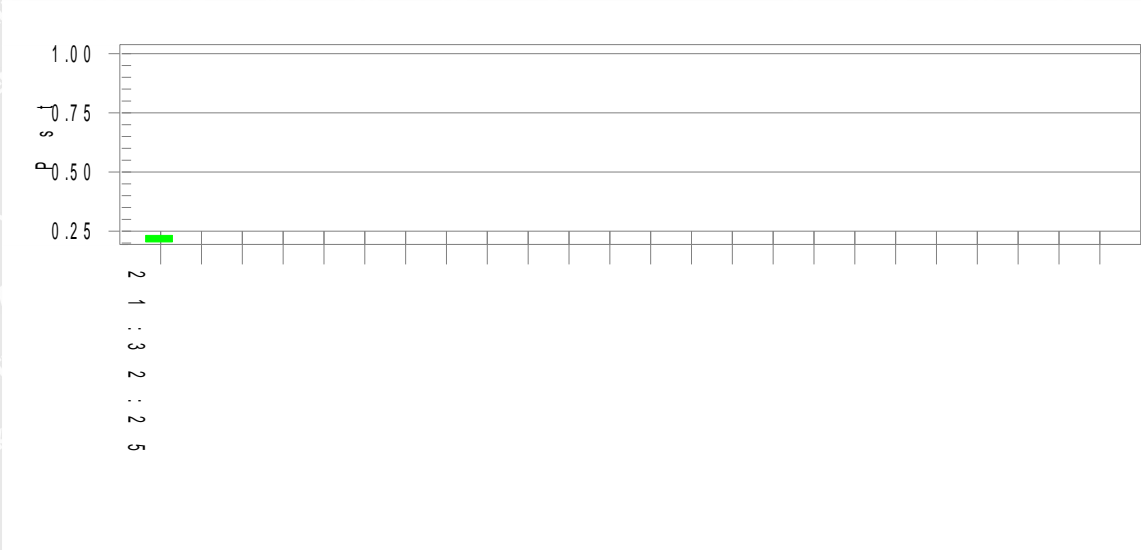
Flicker Test Summary per IEC61000-3-3:2013/AMD1:2017 (Run time)

Test Result: Pass

Status: Test Completed

Pst and limit line

European Limits



Plt and limit line



Parameter values recorded during the test:

Vrms at the end of test (Volt): 230.04

Highest dt (%):

T-max (mS): 0

Highest dc (%): 0.00

Highest dmax (%): 0.00

Highest Pst (10 min. period): 0.233

Highest Plt (2 hr. period): 0.102

Test limit (%):

Test limit (mS): 500.0 Pass

Test limit (%): 3.30 Pass

Test limit (%): 4.00 Pass

Test limit: 1.000 Pass

Test limit: 0.650 Pass

Waltek Testing Group (Shenzhen) Co., Ltd.

[Http://www.waltek.com.cn](http://www.waltek.com.cn)



GTM96300-3624-T2

| | |
|------------|-----|
| Test mode: | TM3 |
|------------|-----|

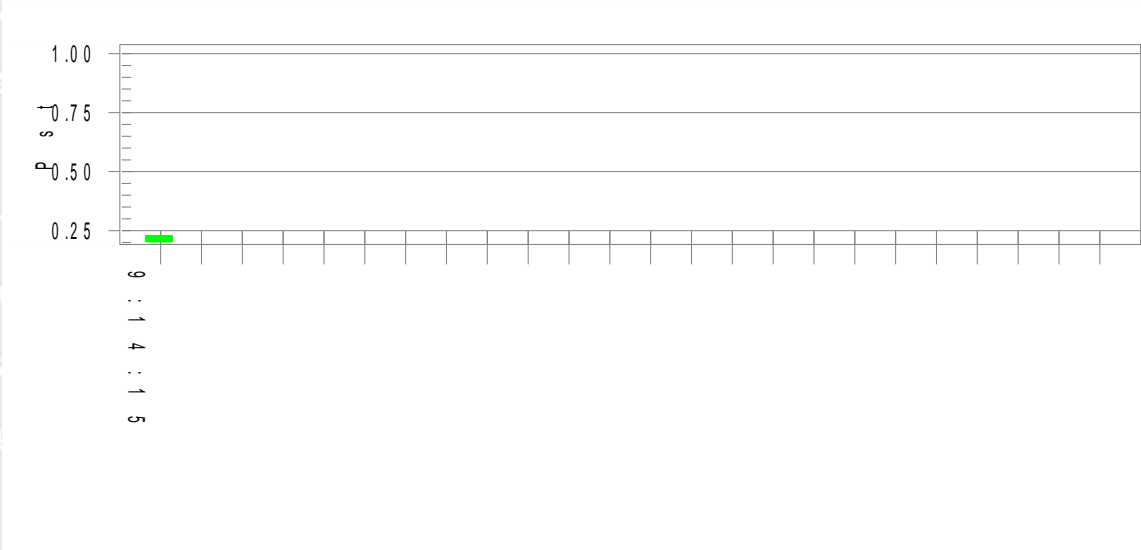
Flicker Test Summary per IEC61000-3-3:2013/AMD1:2017 (Run time)

Test Result: Pass

Status: Test Completed

Pst and limit line

European Limits



Plt and limit line



Parameter values recorded during the test:

Vrms at the end of test (Volt): 229.99

Highest dt (%):

T-max (mS): 0

Highest dc (%): 0.00

Highest dmax (%): 0.00

Highest Pst (10 min. period): 0.230

Highest Plt (2 hr. period): 0.101

Test limit (%):

Test limit (mS): 500.0 Pass

Test limit (%): 3.30 Pass

Test limit (%): 4.00 Pass

Test limit: 1.000 Pass

Test limit: 0.650 Pass

Waltek Testing Group (Shenzhen) Co., Ltd.

[Http://www.waltek.com.cn](http://www.waltek.com.cn)



7. Electrostatic Discharges (ESD)

7.1 Test Procedure

Test is conducted under the description of EN 61000-4-2.


7.2 Test Performance

Performance Criterion: B

7.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 20.5 °C |
| Relative Humidity: | 47 % |
| ATM Pressure: | 1012 mbar |

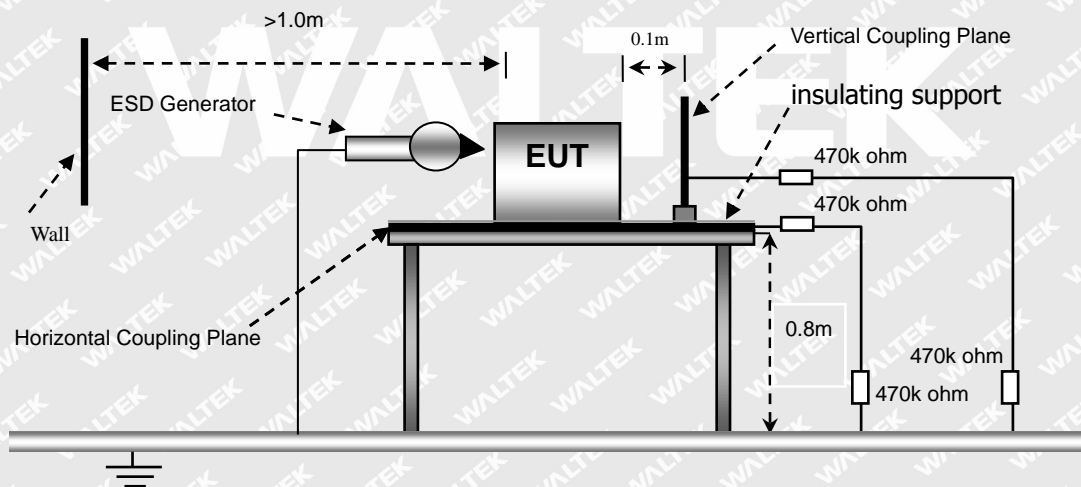7.4 Basic Test Setup Block Diagram





7.5 Electrostatic Discharge Immunity Test Data

TM1/ TM2/ TM3

Table 1: Electrostatic Discharge Immunity (Air Discharge)

| EN 61000-4-2 | Test Voltage (kV) | | | | | | | | | |
|---------------|-------------------|----|----|----|-----|-----|-----|-----|-----|-----|
| Test Points | -4 | +4 | -8 | +8 | -10 | +10 | -16 | +16 | -20 | +20 |
| Surface crack | A | A | A | A | A | A | B | B | B | B |

Table 2: Electrostatic Discharge Immunity (Direct Contact)

| EN 61000-4-2 | Test Voltage (kV) | | | | | | | | | |
|--------------|-------------------|----|----|----|-----|-----|-----|-----|-----|-----|
| Test Points | -4 | +4 | -8 | +8 | -10 | +10 | -16 | +16 | -20 | +20 |
| / | / | / | / | / | / | / | / | / | / | / |

Table 3: Electrostatic Discharge Immunity (Indirect Contact HCP & VCP)

| EN 61000-4-2 | Test Voltage (kV) | | | | | | | | | |
|---------------|-------------------|----|----|----|-----|-----|-----|-----|-----|-----|
| Test Points | -4 | +4 | -8 | +8 | -10 | +10 | -16 | +16 | -20 | +20 |
| HCP (6 Sides) | A | A | A | A | A | A | B | B | B | B |
| VCP (4 Sides) | A | A | A | A | A | A | B | B | B | B |

Test Result: Pass



8. Continuous RF Electromagnetic Field Disturbances (RS)

8.1 Test Procedure

Test is conducted under the description of EN 61000-4-3.


8.2 Test Performance

Performance Criterion: A

8.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 23.0 °C |
| Relative Humidity: | 54 % |
| ATM Pressure: | 1010 mbar |

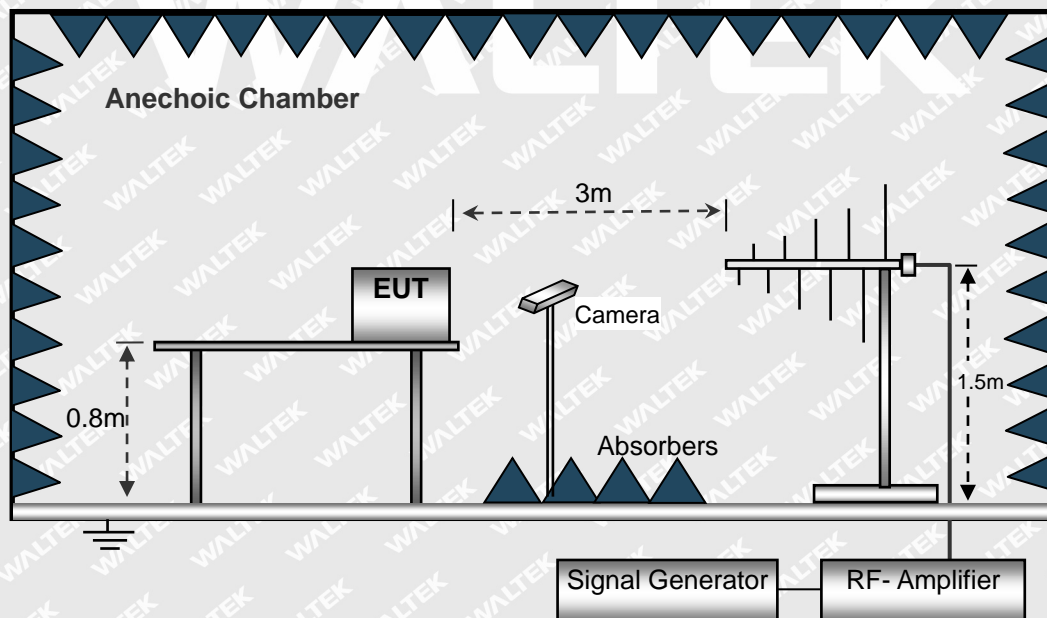8.4 Basic Test Setup Block Diagram





8.5 Continuous Radiated Disturbances Test Data

Frequency step: 1% of fundamental

Dwell time: 1 second

Modulation: AM by 1kHz sine wave with 80% modulation depth

TM1/TM2/TM3

| Frequency Range(MHz) | Field (V/m) | Front | | Rear | | Left Side | | Right Side | |
|----------------------|-------------|-------|------|------|------|-----------|------|------------|------|
| | | VERT | HORI | VERT | HORI | VERT | HORI | VERT | HORI |
| 80-1000 | 10 | A | A | A | A | A | A | A | A |

| Spot frequencies (MHz) | Field (V/m) | Front | | Rear | | Left Side | | Right Side | |
|------------------------|-------------|-------|------|------|------|-----------|------|------------|------|
| | | VERT | HORI | VERT | HORI | VERT | HORI | VERT | HORI |
| 1800 | 10 | A | A | A | A | A | A | A | A |
| 2600 | 10 | A | A | A | A | A | A | A | A |
| 3500 | 10 | A | A | A | A | A | A | A | A |
| 5000 | 10 | A | A | A | A | A | A | A | A |

Test Result: Pass



9. Electrical Fast Transients (EFT)

9.1 Test Procedure

Test is conducted under the description of EN 61000-4-4.


9.2 Test Performance

Performance Criterion: B

9.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 23.5 °C |
| Relative Humidity: | 51 % |
| ATM Pressure: | 1011 mbar |

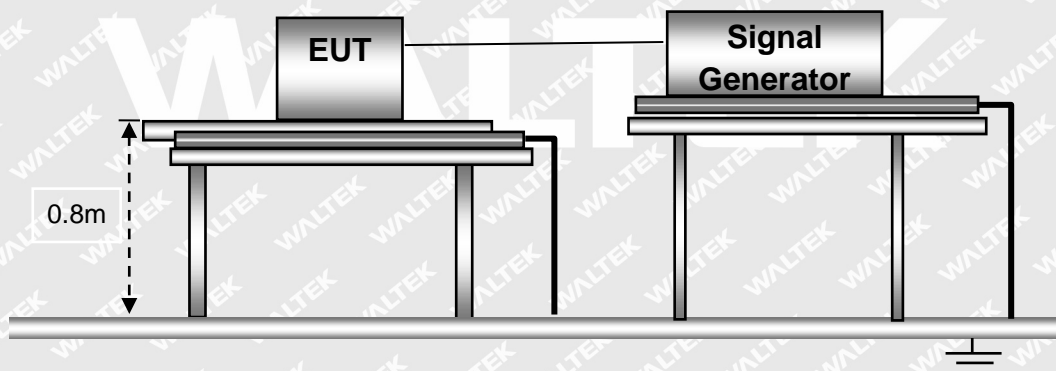9.4 Basic Test Setup Block Diagram





9.5 Electrical Fast Transients Test Data

TM1

| EN 61000-4-4 Test Points | | Test Voltage (kV) | | | | | | | |
|-----------------------------------|----------|-------------------|------|------|------|------|------|------|------|
| | | +0.5 | -0.5 | +1.0 | -1.0 | +2.0 | -2.0 | +4.0 | -4.0 |
| Power Supply Power Port of EUT | L1 | A | A | A | A | B | B | B | B |
| | L2 | A | A | A | A | B | B | B | B |
| | PE | A | A | A | A | B | B | B | B |
| | L1+L2 | A | A | A | A | B | B | B | B |
| | L1 + PE | A | A | A | A | B | B | B | B |
| | L2 + PE | A | A | A | A | B | B | B | B |
| | L1+L2+PE | A | A | A | A | B | B | B | B |
| Signal ports | RJ45 | / | / | / | / | / | / | / | / |

TM2

| EN 61000-4-4 Test Points | | Test Voltage (kV) | | | | | | | |
|-----------------------------------|----------|-------------------|------|------|------|------|------|------|------|
| | | +0.5 | -0.5 | +1.0 | -1.0 | +2.0 | -2.0 | +4.0 | -4.0 |
| Power Supply Power Port of EUT | L1 | A | A | A | A | B | B | B | B |
| | L2 | A | A | A | A | B | B | B | B |
| | PE | A | A | A | A | B | B | B | B |
| | L1+L2 | A | A | A | A | B | B | B | B |
| | L1 + PE | A | A | A | A | B | B | B | B |
| | L2 + PE | A | A | A | A | B | B | B | B |
| | L1+L2+PE | A | A | A | A | B | B | B | B |
| Signal ports | RJ45 | / | / | / | / | / | / | / | / |



TM3

| EN 61000-4-4 Test Points | | Test Voltage (kV) | | | | | | | |
|---------------------------------------|----------|-------------------|------|------|------|------|------|------|------|
| | | +0.5 | -0.5 | +1.0 | -1.0 | +2.0 | -2.0 | +4.0 | -4.0 |
| Power Supply Power Port of EUT | L1 | A | A | A | A | B | B | B | B |
| | L2 | A | A | A | A | B | B | B | B |
| | PE | / | / | / | / | / | / | / | / |
| | L1+L2 | A | A | A | A | B | B | B | B |
| | L1 + PE | / | / | / | / | / | / | / | / |
| | L2 + PE | / | / | / | / | / | / | / | / |
| | L1+L2+PE | / | / | / | / | / | / | / | / |
| Signal ports | RJ45 | / | / | / | / | / | / | / | / |

Test Result: Pass

WALTEK



10. Surges

10.1 Test Procedure

Test is conducted under the description of EN 61000-4-5.


10.2 Test Performance

Performance Criterion: B

10.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 24 °C |
| Relative Humidity: | 51 % |
| ATM Pressure: | 1013 mbar |

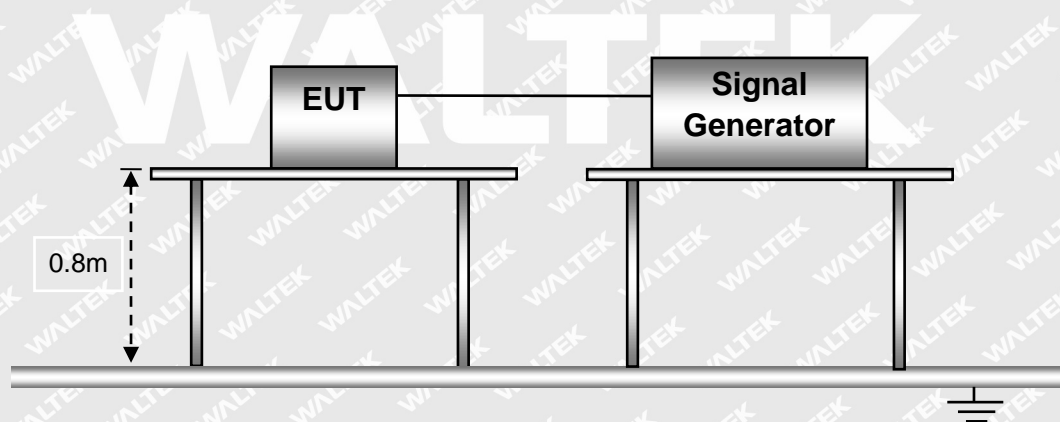10.4 Basic Test Setup Block Diagram





10.5 Surge Test Data

TM1

AC Port

| Test Voltage (kV) | Poll | Path | Pass | Fail |
|-------------------|------|-----------------|------|------|
| 0.5kV | ± | L-N, L-PE, N-PE | A | / |
| 1kV | ± | L-N, L-PE, N-PE | A | / |
| 2kV | ± | L-N, L-PE, N-PE | A | / |
| 4kV | ± | L-N, L-PE, N-PE | A | / |

TM2

AC Port

| Test Voltage (kV) | Poll | Path | Pass | Fail |
|-------------------|------|-----------------|------|------|
| 0.5kV | ± | L-N, L-PE, N-PE | A | / |
| 1kV | ± | L-N, L-PE, N-PE | A | / |
| 2kV | ± | L-N, L-PE, N-PE | A | / |
| 4kV | ± | L-N, L-PE, N-PE | A | / |

TM3

AC Port

| Test Voltage (kV) | Poll | Path | Pass | Fail |
|-------------------|------|------|------|------|
| 0.5kV | ± | L-N | A | / |
| 1kV | ± | L-N | A | / |
| 2kV | ± | L-N | A | / |
| 4kV | ± | L-N | A | / |

Test Result: Pass



11. Continuous Induced RF Disturbances (C/S)

11.1 Test Procedure

Test is conducted under the description of EN 61000-4-6.


11.2 Test Performance

Performance Criterion: A

11.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 23.5 °C |
| Relative Humidity: | 53 % |
| ATM Pressure: | 1013 mbar |

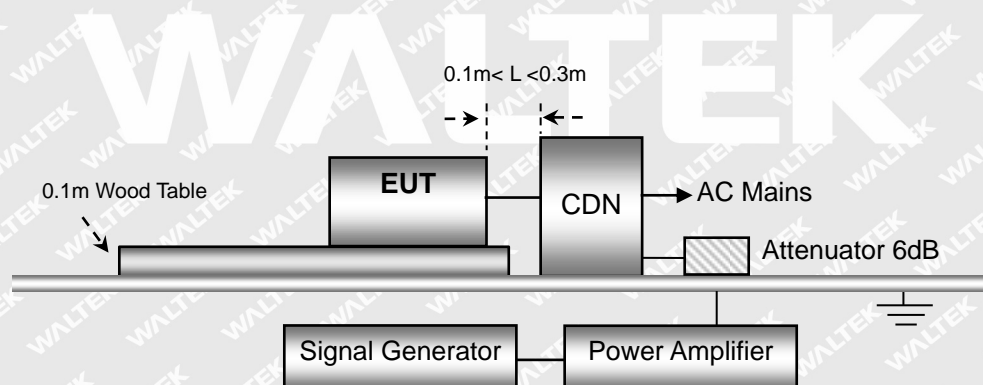11.4 Basic Test Setup Block Diagram





11.5 Continuous Conducted Disturbances Test Data

Sweep frequency range: 0.15MHz to 10MHz 3V; 10MHz to 30MHz 3V to 1V; 30MHz to 80MHz 1V

Frequency step: 1% of fundamental

Dwell time: 1 second

TM1/TM2/TM3

AC Port

| Frequency MHz | Injected Position | Voltage level (e.m.f.) | Observations (Performance Criterion) | Result |
|------------------|-------------------|------------------------------|-----------------------------------------|--------|
| 0.15-80 | AC Mains | 10V | A | Pass |

Test Result: Pass

WALTEK



12. Power-Frequency Magnetic Fields (PFMF)

12.1 Test Procedure

Test is conducted under the description of EN 61000-4-8.


12.2 Test Performance

Performance Criterion: A

12.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 23.0 °C |
| Relative Humidity: | 51 % |
| ATM Pressure: | 1013 mbar |

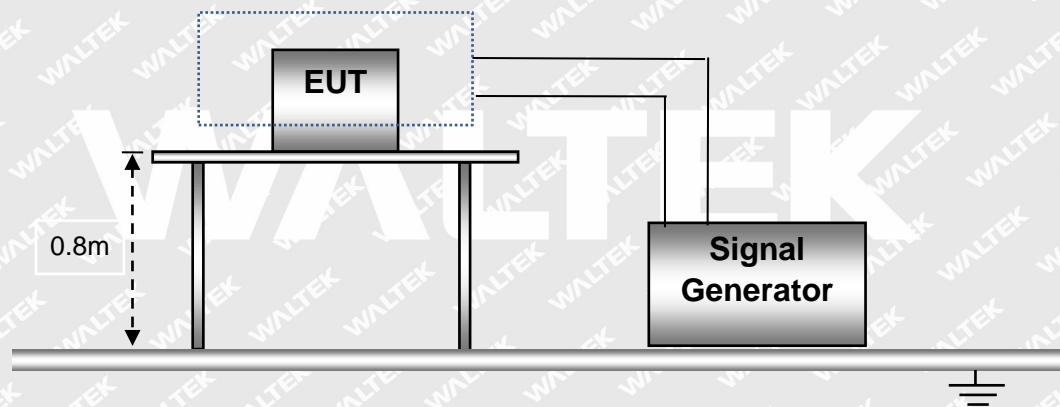12.4 Basic Test Setup Block Diagram



**12.5 Power-Frequency Magnetic Field Test Data**

TM1/TM2/TM3

| Level | Magnetic Field Strength (r.m.s) A/m | Frequency Hz | Induction Coil Position | Pass | Fail |
|-------|-------------------------------------------|-----------------|----------------------------|------|------|
| 1 | 1 | 50 | X, Y, Z | A | / |
| 2 | 3 | 50 | X, Y, Z | A | / |
| 3 | 10 | 50 | X, Y, Z | A | / |
| 4 | 30 | 50 | X, Y, Z | A | / |

Test Result: Pass

WALTEK



13. Voltage Dips and Interruptions

13.1 Test Procedure

Test is conducted under the description of EN 61000-4-11.

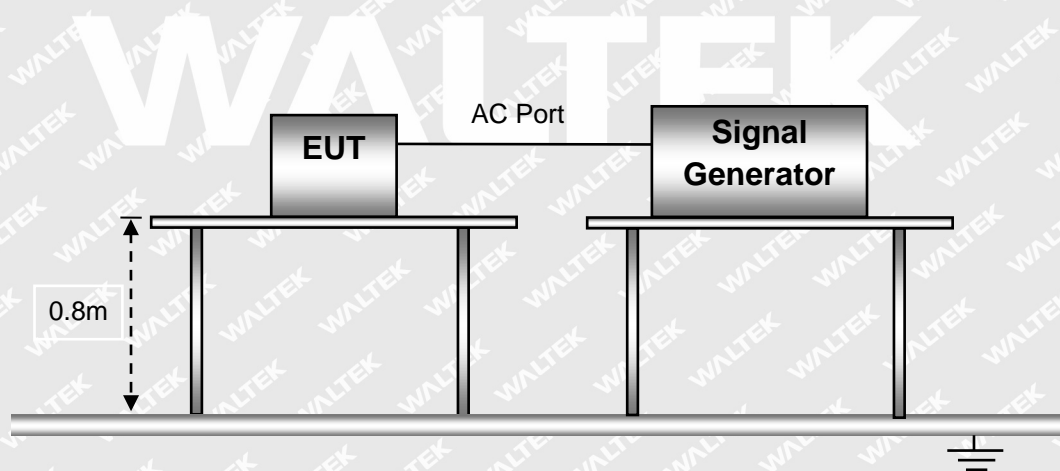
13.2 Test Performance

Performance Criterion: B/C

13.3 Environmental Conditions

| | |
|--------------------|-----------|
| Temperature: | 22.5 °C |
| Relative Humidity: | 51 % |
| ATM Pressure: | 1012 mbar |

13.4 Basic Test Setup Block Diagram





13.5 Voltage Dips And Interruptions Test Data

U: Voltage dips in % U_T (U_T is rated voltage for the EUT)

T: Test duration

TM1/TM2/TM3

| Level | U | T | Phase Angle | N | Pass | Fail |
|-------|------|--------|--------------|---|------|------|
| 1 | 100% | 10ms | 0/90/180/270 | 3 | B | / |
| 2 | 30% | 500ms | 0/90/180/270 | 3 | B | / |
| 3 | 100% | 5000ms | 0/90/180/270 | 3 | B | / |



Test Result: Pass

WALTEK



EXHIBIT 1 - PRODUCT LABELING

Proposed CE Label Format

| | |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Medical/ITE Power Supply | |
| Model: GTM96180-1811-2.0-T3, GTM91120-3024-T3A, GTM96300-3624-T2 | |
| Brand: |  |
| Importer Name: | XXX |
| Importer Address: | XXX |
| 1. GlobTek, Inc. 2. GlobTek (Suzhou) Co., Ltd 1.186 Veterans Dr. Northvale, NJ 07647 USA 2. Building 4, No. 76, Jin Ling East Rd., Suzhou Industrial Park, Suzhou, JiangSu 215021, China | |
| |   |

Specifications: Text is Black in color and is justified. Labels are printed in indelible ink on permanent adhesive backing or silk-screened onto the EUT or shall be affixed at a conspicuous location on the EUT. The 'CE' marking must be affixed to the EUT or to its data plate. Where this is not possible or not warranted on account of the nature of the apparatus, it must be affixed to the packaging, if any, and to the accompanying documents. The 'CE' marking is allowed less than 5 mm but must clear. If the 'CE' marking is reduced or enlarged the proportions given in the above graduated drawing must be respected. The Importer name, address and Manufacturer name and address should indicate on marking label or packaging or in a document accompanying.

Proposed Label Location on EUT

CE Label Location





EXHIBIT 2 - EUT PHOTOGRAPHS

GTM96180-1811-2.0-T3

EUT View 1



EUT View 2





EUT View 3



EUT View 4





GTM91120-3024-T3A
EUT View 1



EUT View 2





EUT View 3

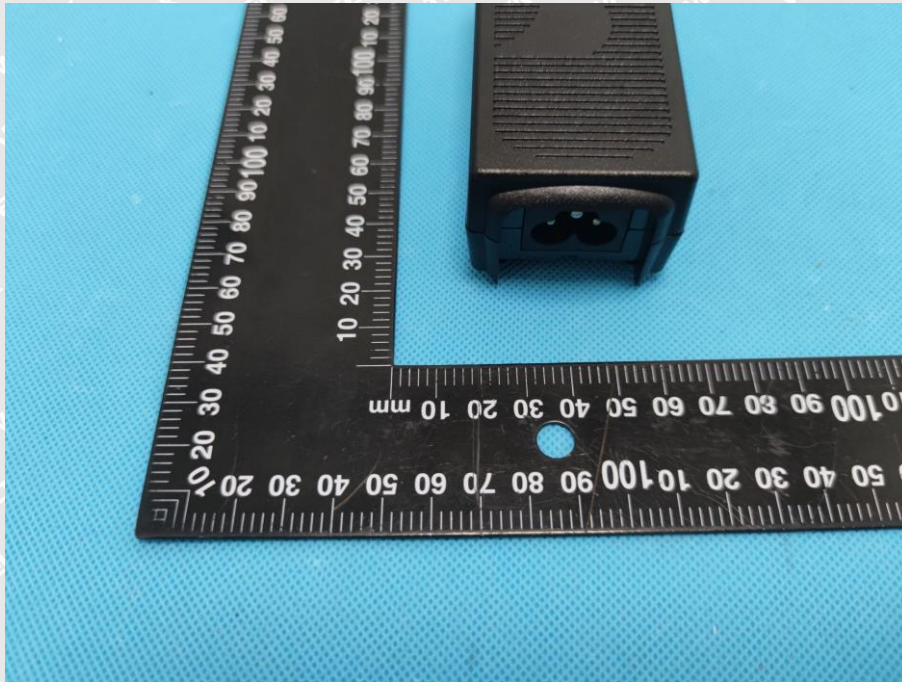


EUT View 4





EUT View 5



WALTEK



GTM96300-3624-T2
EUT View 1

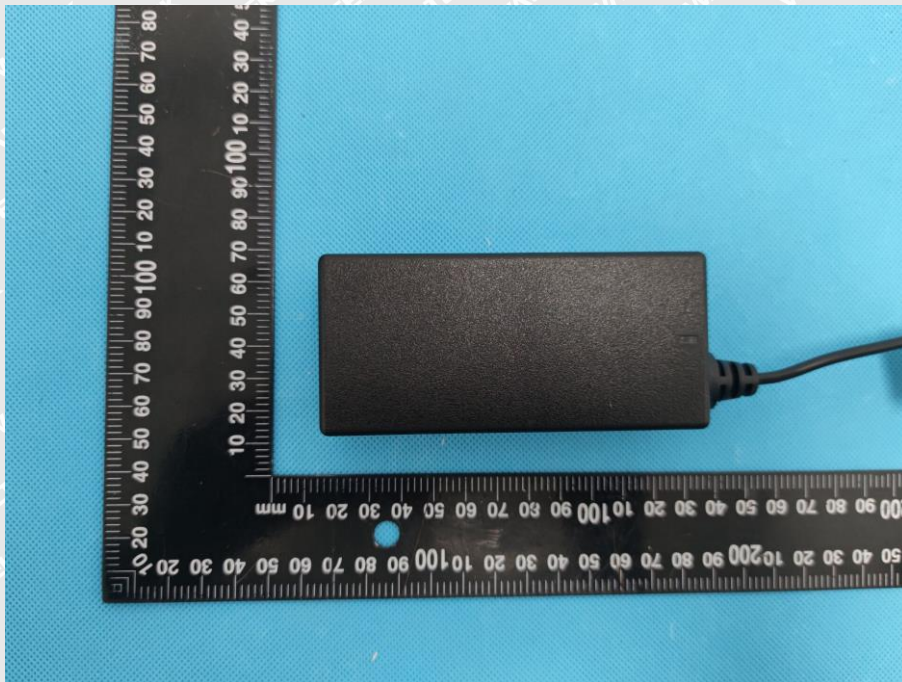


EUT View 2





EUT View 3




EUT View 4





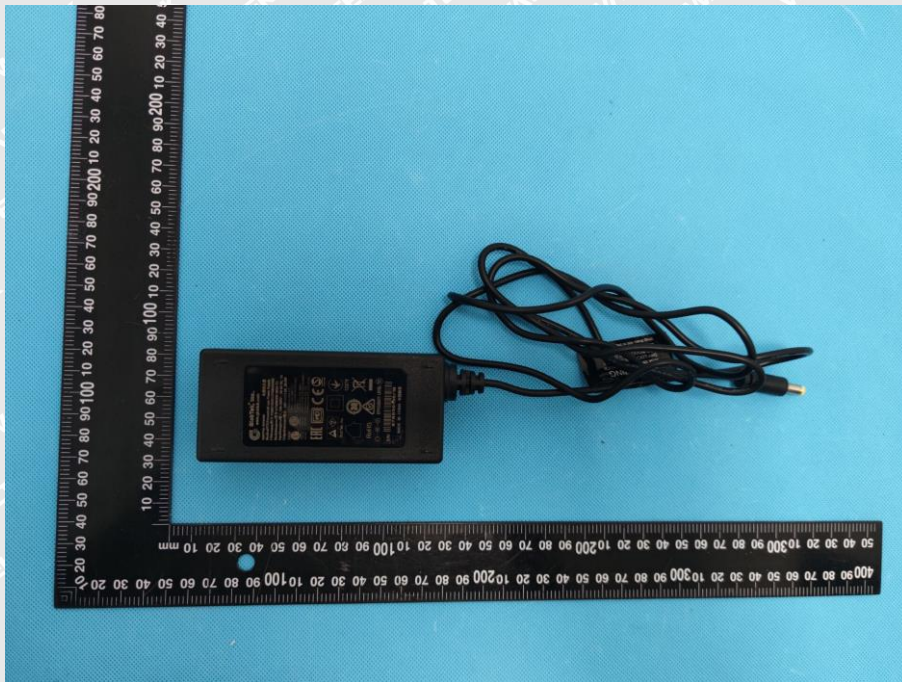EUT View 5




WALTEK




GTM96180-1811-2.0-T3

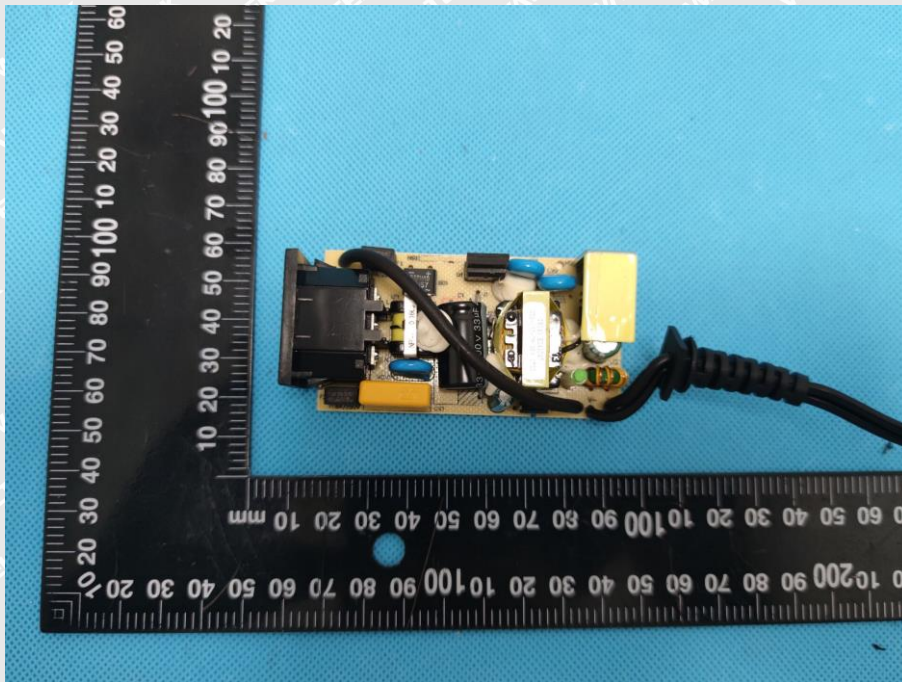Solder Board-Component View 1




Solder Board-Component View 2

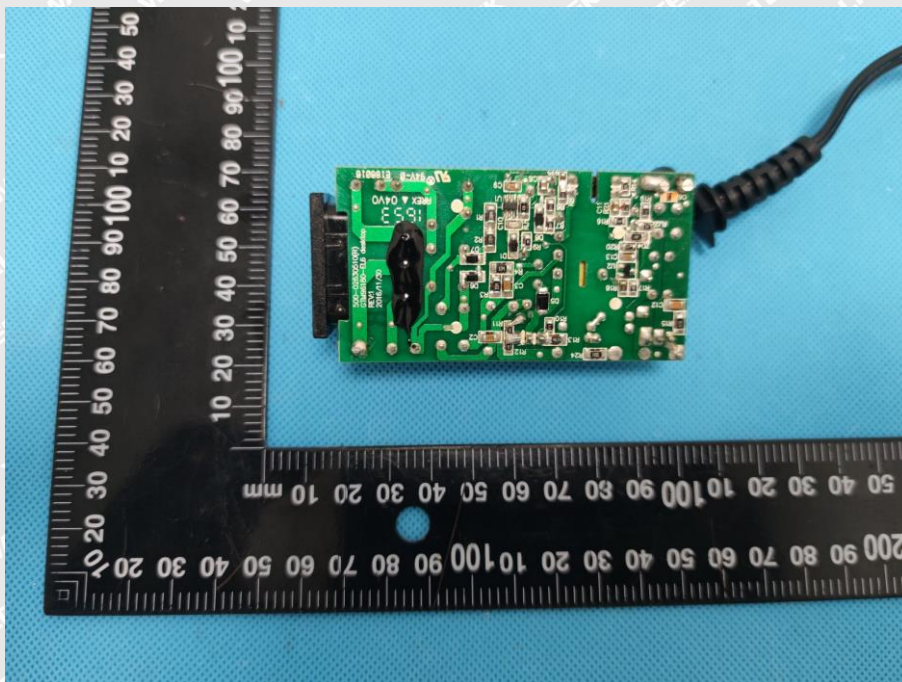




GTM91120-3024-T3A

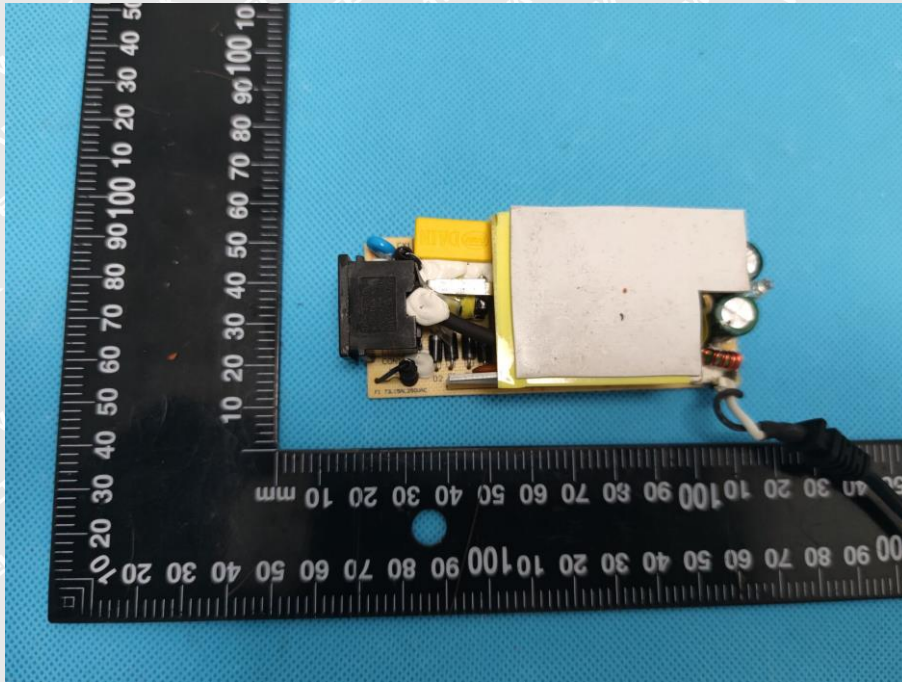Solder Board-Component View 1




Solder Board-Component View 2

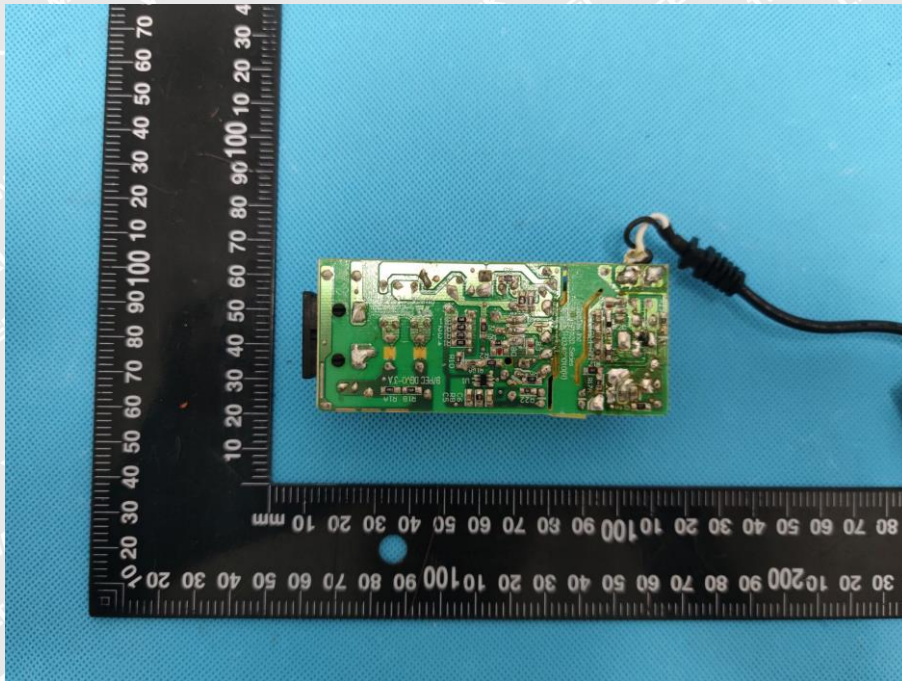



GTM96300-3624-T2

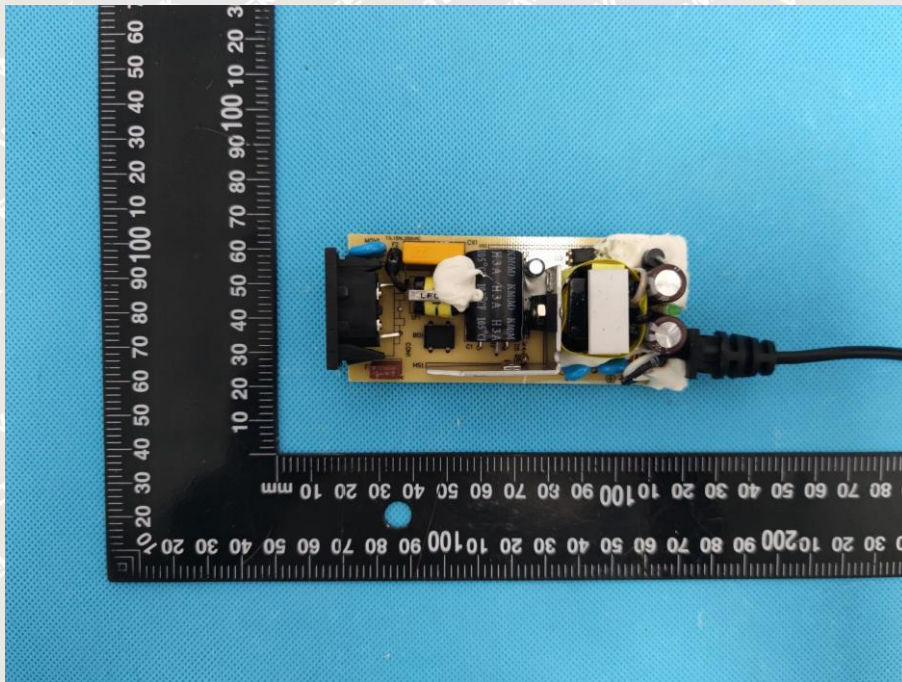Solder Board-Component View 1



Solder Board-Component View 2

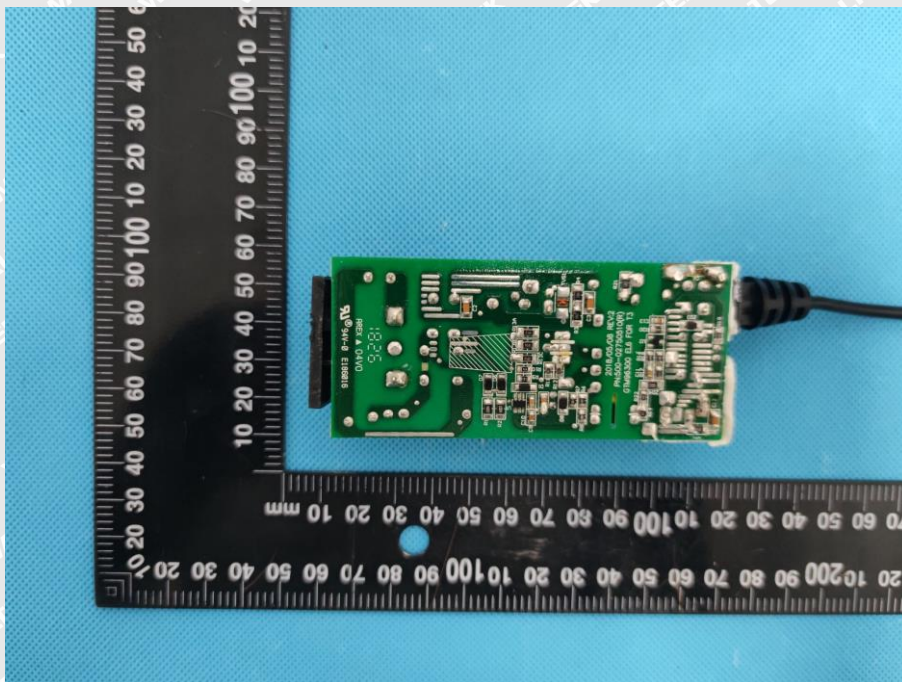
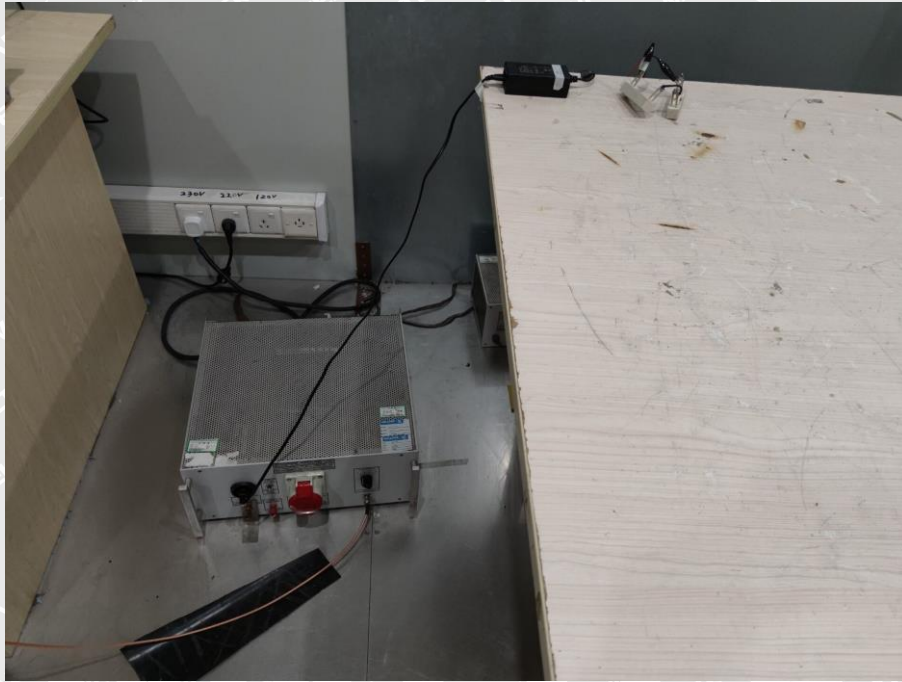


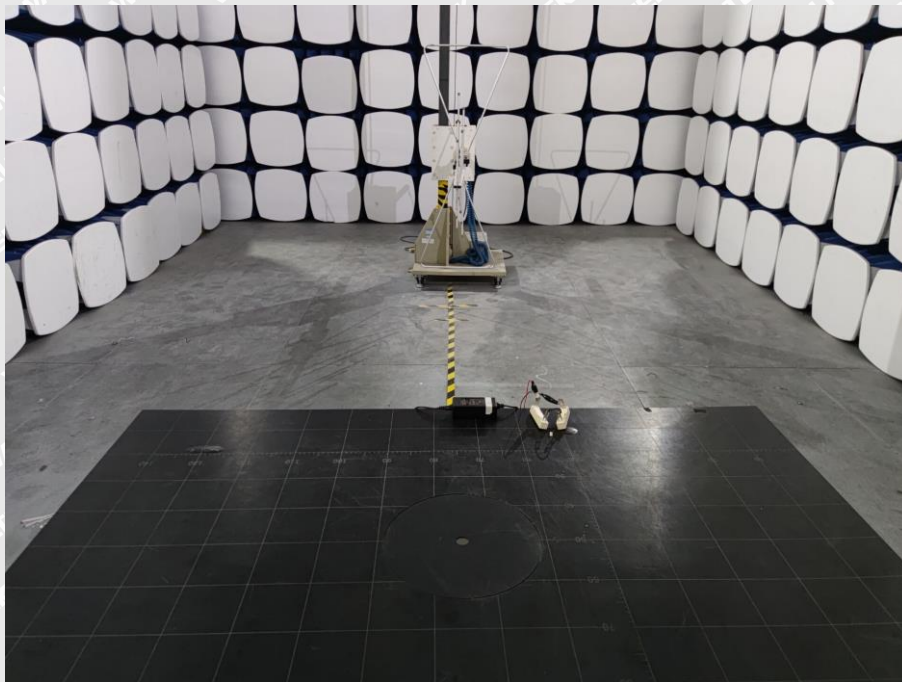


EXHIBIT 3 - TEST SETUP PHOTOGRAPHS

Conduction Emission Test View TM1



Radiation Emission Test View TM1






Harmonic/Flicker Test View TM1




WALTEK

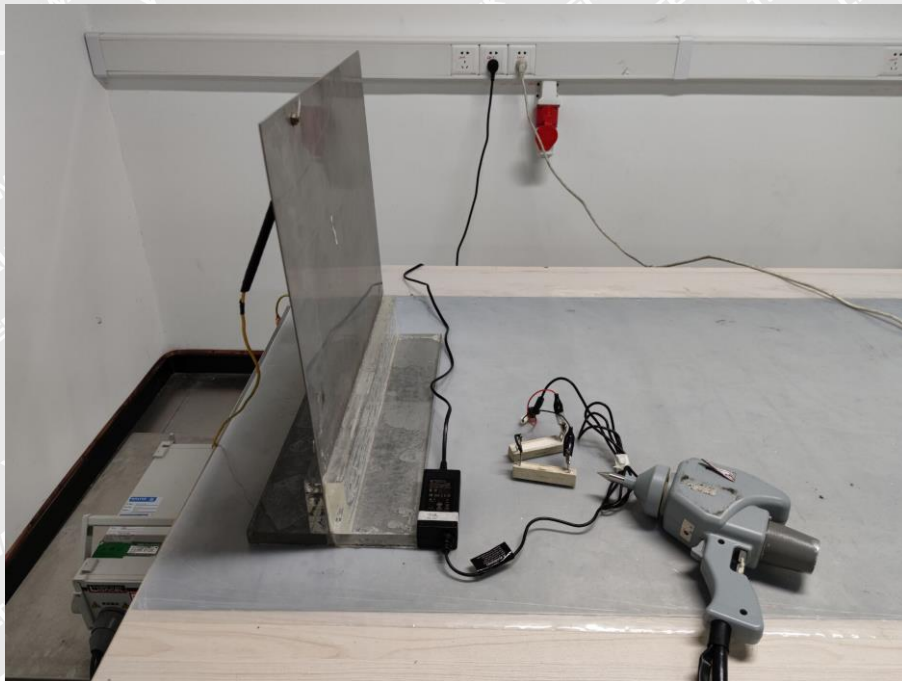EN 61000-4-2 Test View TM1






EN 61000-4-3 Test View TM1

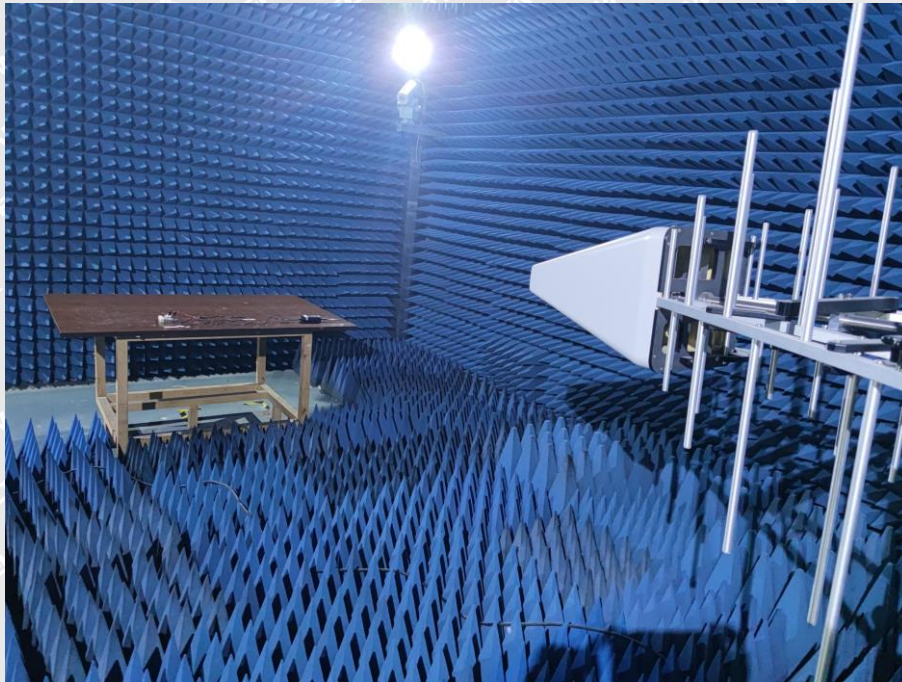


EN 61000-4-4/5/11 Test View TM1

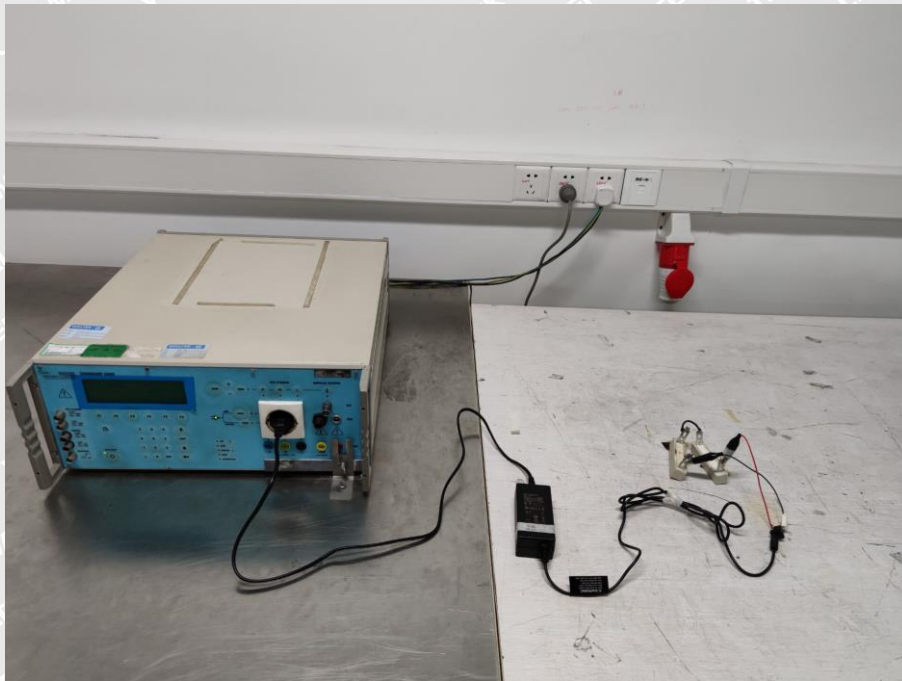




EN 61000-4-6 Test View TM1

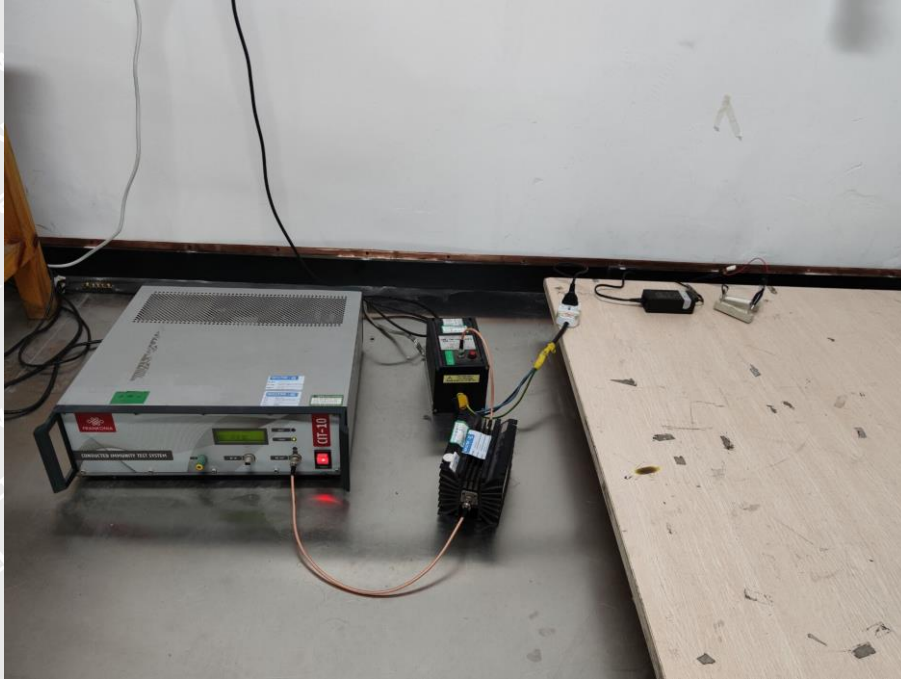

EN 61000-4-8 Test View TM1

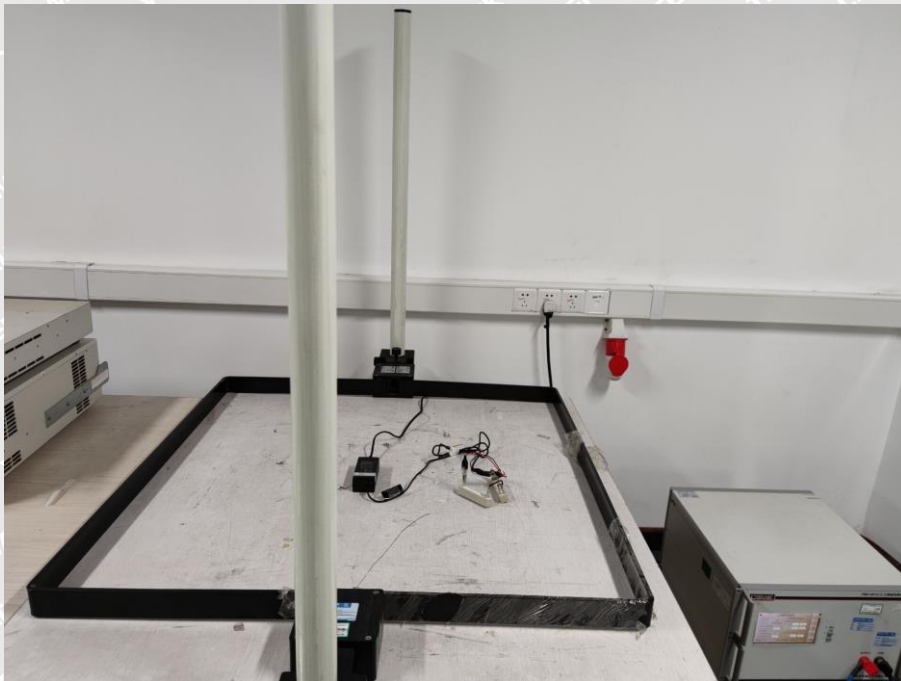




Conduction Emission Test View TM2




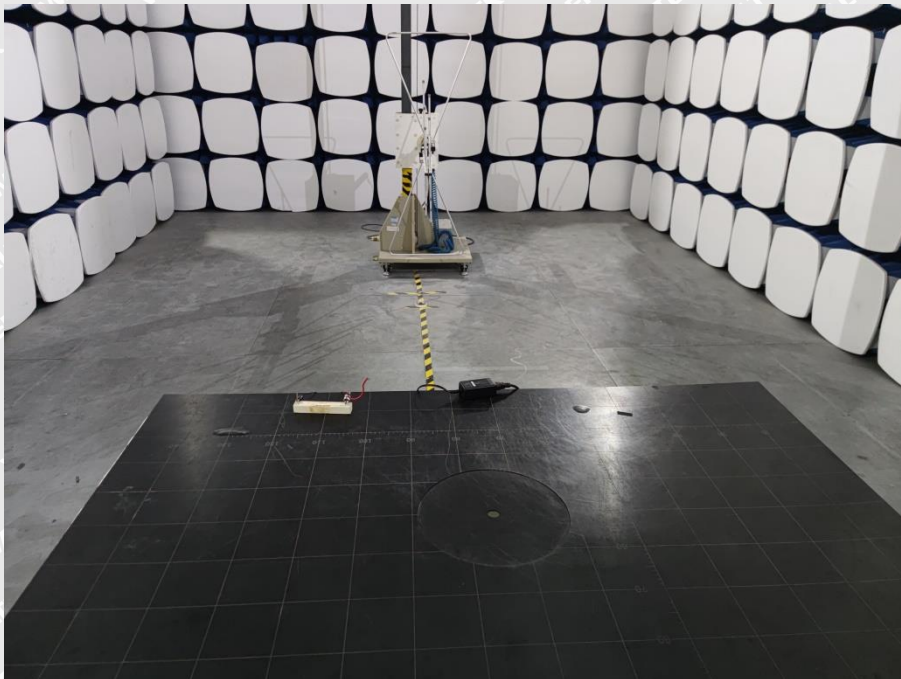Radiation Emission Test View TM2






Harmonic/Flicker Test View TM2

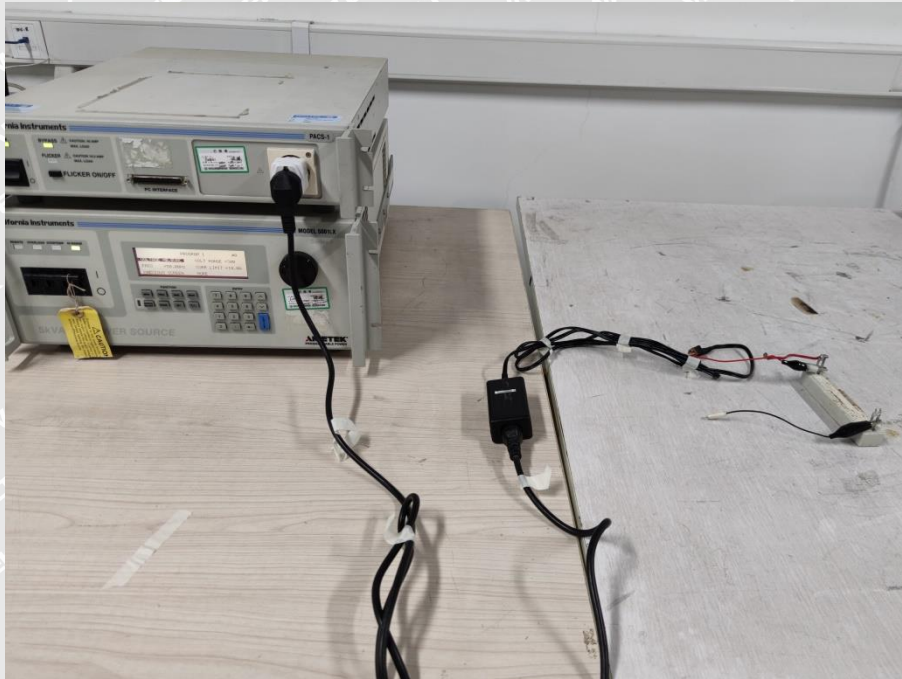


EN 61000-4-2 Test View TM2

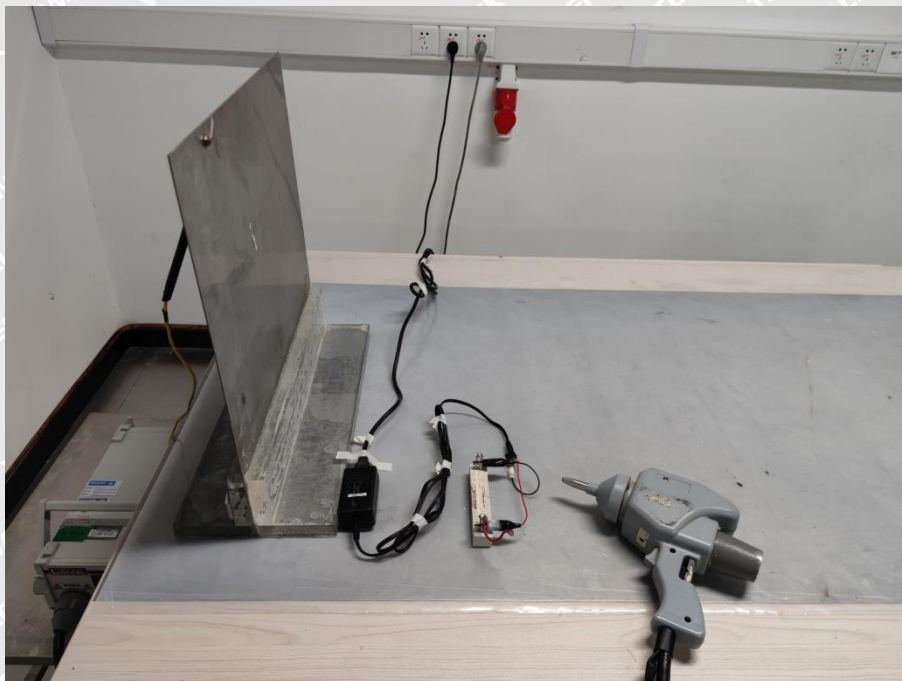




EN 61000-4-3 Test View TM2

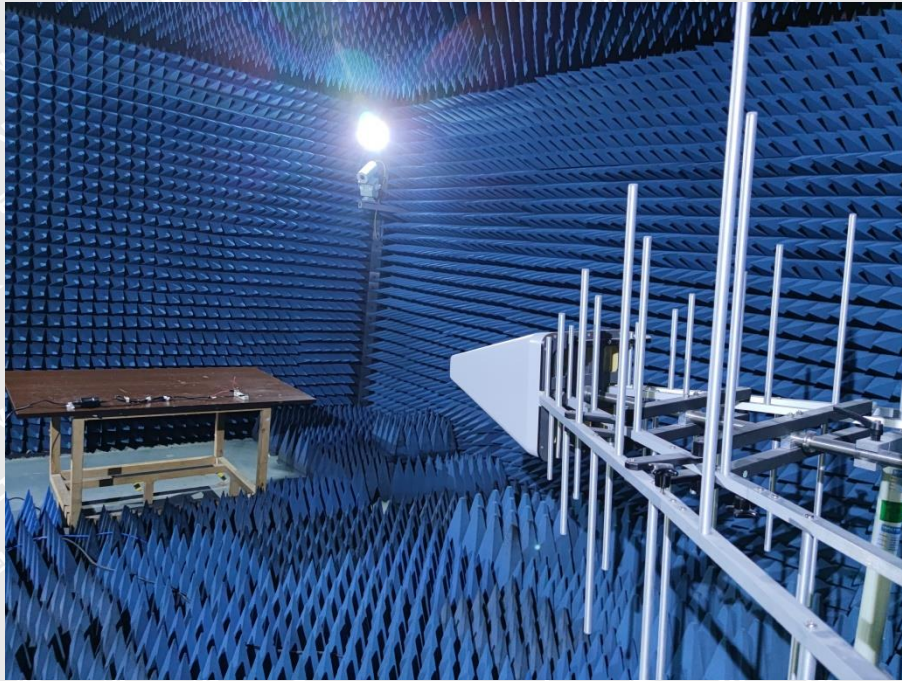


WALTEK

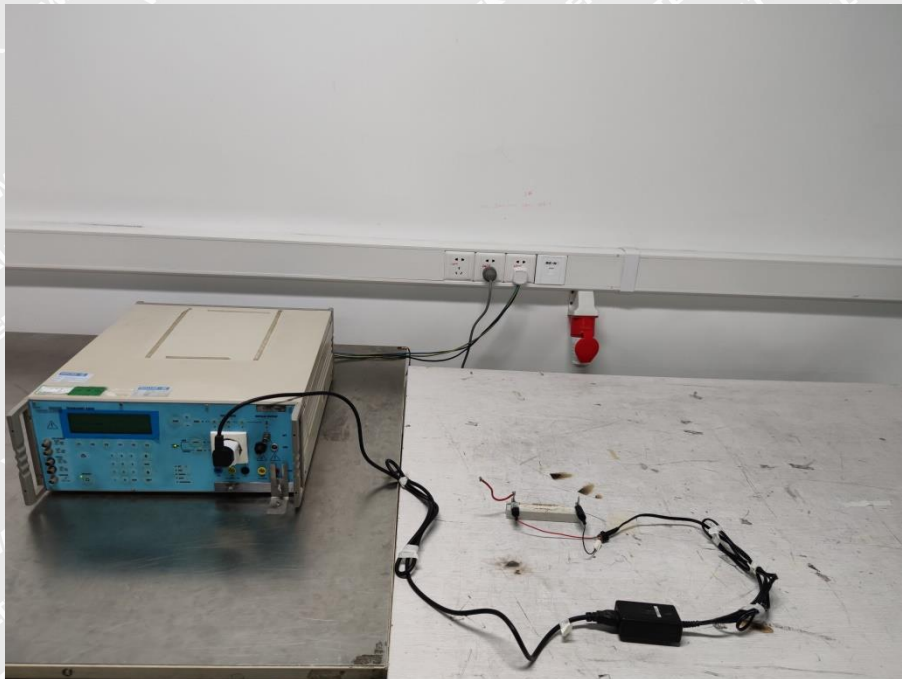EN 61000-4-4/5/11 Test View TM2






EN 61000-4-6 Test View TM2

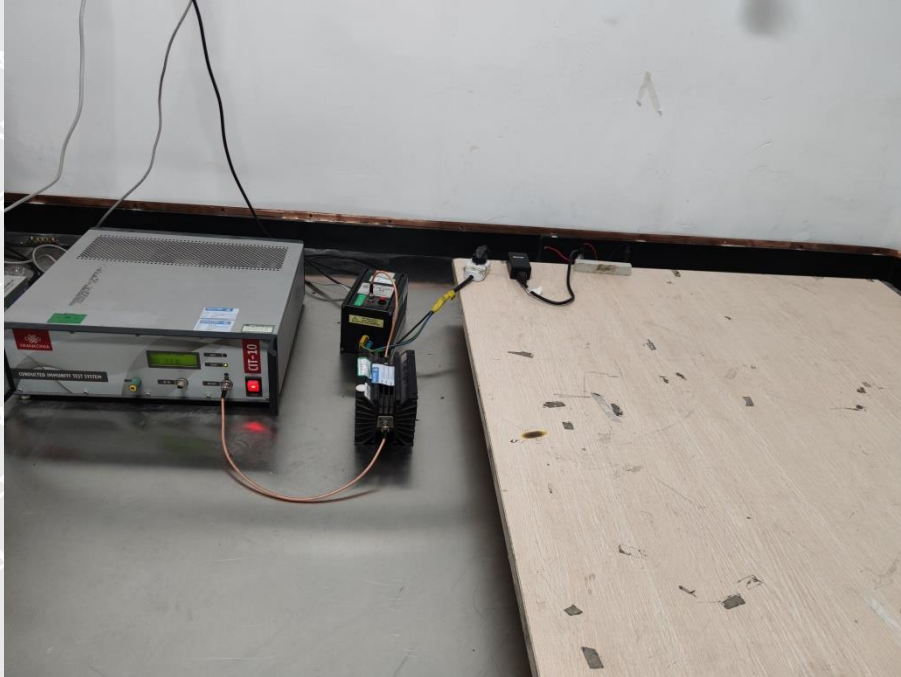

EN 61000-4-8 Test View TM2

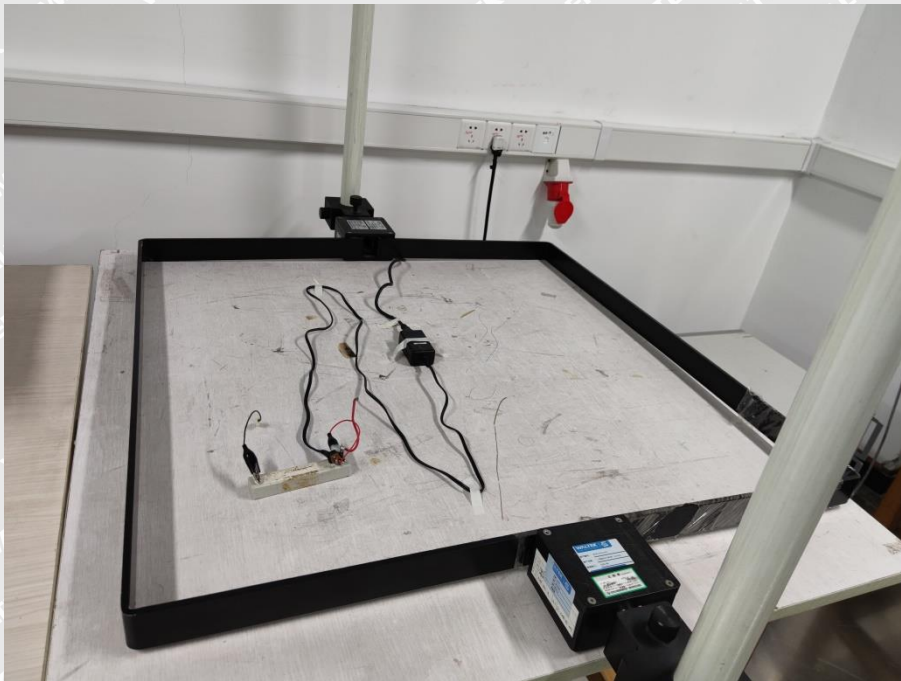

***** END OF REPORT *****