



Test Report issued under the responsibility of:



IEC 60601-1
Medical electrical equipment

Part 1: General requirements for basic safety and essential performance

Report Reference No......: **T223-0388/12**
Date of issue: **2012-10-29**
Total number of pages: **266 pages**

CB Testing Laboratory.....: **SIQ – Slovenian Institute of Quality and Metrology**
Testing Laboratory is accredited by Slovenian Accreditation, Reg. No.: LP-009
Address: **Tržaška cesta 2, 1000 Ljubljana, Slovenia**

Applicant's name.....: **GlobTek, Inc.**
Address: **186 Veterans Drive Northvale, NJ 07647, USA**

Test specification:
Standard: **IEC 60601-1: 2005 + CORR. 1 (2006) + CORR. 2 (2007)**
Test procedure.....: **CB Scheme**
Non-standard test method.....: **N/A**

Test Report Form No......: **IEC60601_1G**
Test Report Form Originator: **Underwriters Laboratories Inc.**
Master TRF: **Dated 2010-11**

Copyright © 2010 IEC System for Conformity Testing and Certification of Electrical Equipment (IECEE), Geneva, Switzerland. All rights reserved.

This publication may be reproduced in whole or in part for non-commercial purposes as long as the IECEE is acknowledged as copyright owner and source of the material. IECEE takes no responsibility for and will not assume liability for damages resulting from the reader's interpretation of the reproduced material due to its placement and context.

If this Test Report Form is used by non-IECEE members, the IECEE/IEC logo shall be removed

This report is not valid as a CB Test Report unless signed by an approved CB Testing Laboratory and appended to a CB Test Certificate issued by an NCB in accordance with IECEE 02.

Test item description: **Switch Mode Power Supply Unit for Building-in**
Trade Mark: **GlobTek**
Manufacturer.....: **GlobTek, Inc.**
186 Veterans Drive Northvale, NJ 07647, USA
Model/Type reference.....: **GTM2065yyzz-X.X-F; GTM2065yyzz-X.X-FA**
-X.X is optional and denotes voltage differentiator X.X from rated voltage
“yy” means output power in Watts
“zz” means output voltage in Volts
See next page for details.

Ratings : I/P: 100-240 V~; 50-60 Hz; 1500-800 mA



O/P: See below

Standard 65 W output models (without air flow):

Model name	Output voltage (Vdc)	Output current (A)
GTM2065-333.3-F	3,3 Vdc	9,70 A
GTM2065-4005-F	5,0 Vdc	8,00 A
GTM2065-657.5-F	7,5 Vdc	8,67 A
GTM2065-6509-F	9,0 Vdc	7,22 A
GTM2065-6512-F	12,0 Vdc	5,42 A
GTM2065-6515-F	15,0 Vdc	4,33 A
GTM2065-6518-F	18,0 Vdc	3,61 A
GTM2065-6524-F	24,0 Vdc	2,71 A
GTM2065-6536-F	36,0 Vdc	1,80 A
GTM2065-6548-F	48,0 Vdc	1,36 A

Standard 80 W output models (with 10 CFM air flow):

Model name	Output voltage (Vdc)	Output current (A)
GTM2065-553.3-FA	3,3 Vdc	16,67 A
GTM2065-5505-FA	5,0 Vdc	11,00 A
GTM2065-707.5-FA	7,5 Vdc	9,33 A
GTM2065-8009-FA	9,0 Vdc	8,89 A
GTM2065-8012-FA	12,0 Vdc	6,67 A
GTM2065-8015-FA	15,0 Vdc	5,33 A
GTM2065-8018-FA	18,0 Vdc	4,44 A
GTM2065-8024-FA	24,0 Vdc	3,33 A
GTM2065-8036-FA	36,0 Vdc	2,22 A
GTM2065-8048-FA	48,0 Vdc	1,67 A

Testing procedure and testing location:	
<input checked="" type="checkbox"/> CB Testing Laboratory:	SIQ – Slovenian Institute of Quality and Metrology
Testing location/ address	Tržaška cesta 2, 1000 Ljubljana, Slovenia
<input type="checkbox"/> Associated CB Test Laboratory:	
Testing location/ address	
Tested by (name + signature).. :	Janez Vidmar 
Approved by (+ signature)..... :	Boštjan Glavič 
<input type="checkbox"/> Testing procedure: TMP	
Tested by (name + signature).. :	
Approved by (+ signature)..... :	
Testing location/ address	
<input type="checkbox"/> Testing procedure: WMT	
Tested by (name + signature).. :	
Witnessed by (+ signature)..... :	
Approved by (+ signature)..... :	
Testing location/ address	
<input type="checkbox"/> Testing procedure: SMT	
Tested by (name + signature).. :	
Approved by (+ signature)..... :	
Supervised by (+ signature) :	
Testing location/ address	
<input type="checkbox"/> Testing procedure: RMT	
Tested by (name + signature).. :	
Approved by (+ signature)..... :	
Supervised by (+ signature) :	
Testing location/ address	

List of Attachments (including a total number of pages in each attachment):

1. Test Report (213 pages)
2. National Differences to IEC 60601-1:2005 – Enclosure No. 1 (13 pages)
3. Photo documentation – Enclosure No. 1 (4 pages)
4. Schematics, layouts and documentation – Enclosure No. 2 (36 pages)

Summary of testing:
Tests performed (name of test and test clause):

See next pages

The risk management requirements of the standard were not addressed.

Testing location:

SIQ – Slovenian Institute of Quality and Metrology

Tržaška cesta 2, 1000 Ljubljana, Slovenia

Summary of compliance with National Differences (See enclosure No. 1 for details)

List of countries addressed:

- **US NATIONAL DIFFERENCES** to IEC 60601-1 Third edition
National standard ANSI/AAMI ES60601-1: 2005

- **CANADA NATIONAL DIFFERENCES** to IEC 60601-1 Third edition
National standard CAN/CSA-C22.2 No. 60601-1:08

- **SWITZERLAND NATIONAL DIFFERENCES** to IEC 60601-1 Third edition
National standard SN EN 60601-1:06

Copy of marking plate (example):

The artwork below may be only a draft. The use of certification marks on a product must be authorized by the respective NCBs that own these marks.



XXXX - USA OR CHINA

Tests performed (name of test and test clause):		Verdict
4.11	Power Input	P
7.1.3	Durability of marking	P
8.4	Limitation of voltage current and energy	P
8.5.5.	Defibrillation- proof applied parts	N/A
8.6.4.	Impedance and current- carrying capability of protective earth connections	P
8.7.4.5	Earth Leakage Current	P
8.7.4.6.	Touch Current	P
8.7.4.7.	Patient Leakage Current	N/A
8.7.4.8.	Patient Auxiliary Current	N/A
8.7.4.9.	Multiple Patient Connections	N/A
8.8.3A	Dielectric Strength test of solid insulation materials with safety functions- MOOP	P
8.8.3B	Dielectric Strength test of solid insulation materials with safety functions- MOPP	N/A
8.9.2	Short circuits in Mains part over creepage and clearance distances	P
8.9.3.2	Thermal Cycling Test on one sample of insulation compound forming solid insulation between conductive parts	N/A
8.9.3.4	Thermal Cycling test on one Sample of Cemented joint	N/A
9.2.2.2	Measurement of gap “a” according to table 20 (ISO 13452:1996)	N/A
10.1.1	Measurement of X- radiation	N/A
11.1	Excessive temperatures in ME EQUIPMENT	P
11.2.2.1	Existence of ignition sources	N/A
13.1	Power or energy dissipation	N/A
13.2	Single Fault conditions	P
15.3	Mechanical strength	N/A
15.4.6	Actuating parts of controls	N/A
15.5.1.2	Transformer short circuit	P
15.5.1.3	Transformer overload	P
15.5.2	Transformer dielectric strength after humidity preconditioning of 5.7	N/A
--	Working voltage Measurement	P
--	Evaluation of voltage limiting components in SELV circuits	P

GENERAL INFORMATION	
Test item particulars (see also Clause 6):	
Classification of installation and use..... :	Power supply unit is intended for building-in within end medical product.
Device type (component/sub-assembly/ equipment/ system)..... :	Component level power supply unit for building-in.
Intended use (Including type of patient, application location)..... :	EUT is intended to provide power to medical devices with isolation grade MOOP (Means of Operator Protection)
Mode of operation	Continuous operation
Supply connection	Input connector
Accessories and detachable parts included	No accessories and detachable parts included.
Other options include	No other options included
Testing	
Date of receipt of test item(s)..... :	2010-02-01, 2011-07-04, 2011-09-09, 2012-02-09, 2012-09-11
Dates tests performed	From 2011-09-09 to 2012-10-10
Possible test case verdicts:	
- test case does not apply to the test object	N/A
- test object does meet the requirement..... :	Pass (P)
- test object was not evaluated for the requirement	N/E
- test object does not meet the requirement	Fail (F)
Abbreviations used in the report:	
- normal condition	N.C.
- single fault condition..... :	S.F.C.
- means of Operator protection	MOOP
- means of Patient protection ... :	MOPP
General remarks:	
<p>"(see Attachment #)" refers to additional information appended to the report.</p> <p>"(see appended table)" refers to a table appended to the report.</p> <p>The tests results presented in this report relate only to the object tested.</p> <p>This report shall not be reproduced except in full without the written approval of the testing laboratory.</p> <p>List of test equipment must be kept on file and available for review.</p> <p>Additional test data and/or information provided in the attachments to this report.</p> <p>Throughout this report a <input checked="" type="checkbox"/> comma / <input type="checkbox"/> point is used as the decimal separator.</p>	

Manufacturer's Declaration per sub-clause 6.2.5 of IEC60060-2:

The application for obtaining a CB Test Certificate includes more than one factory location and a declaration from the Manufacturer stating that the sample(s) submitted for evaluation is (are) representative of the products from each factory has been provided : ☒ Yes ☐ Not applicable

When differences exist; they shall be identified in the General product information section.

Name and address of factory (ies) : 1) Globtek, Inc.
186 Veterans Drive Northvale, NJ 07647, USA
2) Globtek (Suzhou) Co., Ltd.
Building 4, No. 76, Jinling East Road, Suzhou Industrial Park, Jiangsu 215021, China

General product information:

The Power Supply GTM2065 series has been designed for the supplying various medical devices with integrated MOOP isolation (Means of Operator Protection).

The Power Supply GTM2065 series is intended for building-in within end medical product.

Power supply is not intended for direct patient connection.

The power supply unit is provided without external enclosure (end product consideration).

Power supply unit is provided with power "ON" indicator provided on the secondary side of the power supply unit.

The power supply in maintenance free.

The power supply is intended for operating at ambient temperature up to 45°C (for models without air flow) or 50°C (for models with 10 CFM air flow. Unit was cooled with fan (airflow 10 CFM), placed on the transformer (T1) side of the power supply, so the direction of the airflow was towards the transformer T1.

The unit shall not be used for use in an oxygen rich environment.

The unit it is not intended to be use with flammable anaesthetics and not intended for use in conjunction with flammable agents.

Power supply unit can be provided with or without protective earth:

- With protective earth: PE conductor provided between J7A and J7B. Functionally isolated metal shield provided on bottom side of the power supply unit. Power supply unit is classified as safety Class I.

- Without protective earth: No PE conductor, no metal shield provided. PE terminal EC1, capacitors CY1, CY2, CY5, CY6, CY7 and CY8 removed from PCB. Power supply unit complies with Class II construction. Safety Class is end product consideration.

Summary of testing:

The component was tested according to the standard IEC 60601-1:2005 (3rd Edition) and/or EN 60601-1:2006 + A11:2011.

The risk management requirements of the standard were not addressed. The power supply tested in this test report is only component level power supply. Risk management shall be addressed to the end type medical equipment.

Essential performance shall be determined within the end medical equipment; however for this medical power supply essential performance is considered MOOP. MOOP is tested within this test report.

The unit is power supply unit intended for building-in within end medical product.

Power supply unit provides internally two fuses in both supply leads:

- Standard 65 W output models (without air flow): T2.0A 250Vac
- Standard 80 W output models (with 10 CFM air flow): T3.15A 250Vac

Power supply unit was evaluated only for Means of Operator Protection:

- 2 x MOOP between primary and secondary circuit
- 2 x MOOP between primary and functionally earthed metal shield
- 1 x MOOP between primary and protective earth

Secondary output circuit is separated from mains by reinforced insulation and rated SELV. The output does not provide hazard energy level.

Power supply is provided with user instruction related to the user and technical specification related to the service personnel.

The power supply is rated as class I or end product consideration (power supply unit complies with Class II construction).

Mains transformer provides reinforced insulation between primary and secondary circuit. This transformer is built up to fulfil the requirement of insulation class B. See also list of safety critical components.


The equipment has been evaluated for use in a Pollution Degree 2 and overvoltage category II environment and a maximum altitude of 2000 m.

Cleaning and disinfection shall be considered within end product investigation.

Disconnecting device is end product consideration.

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

INSULATION DIAGRAM

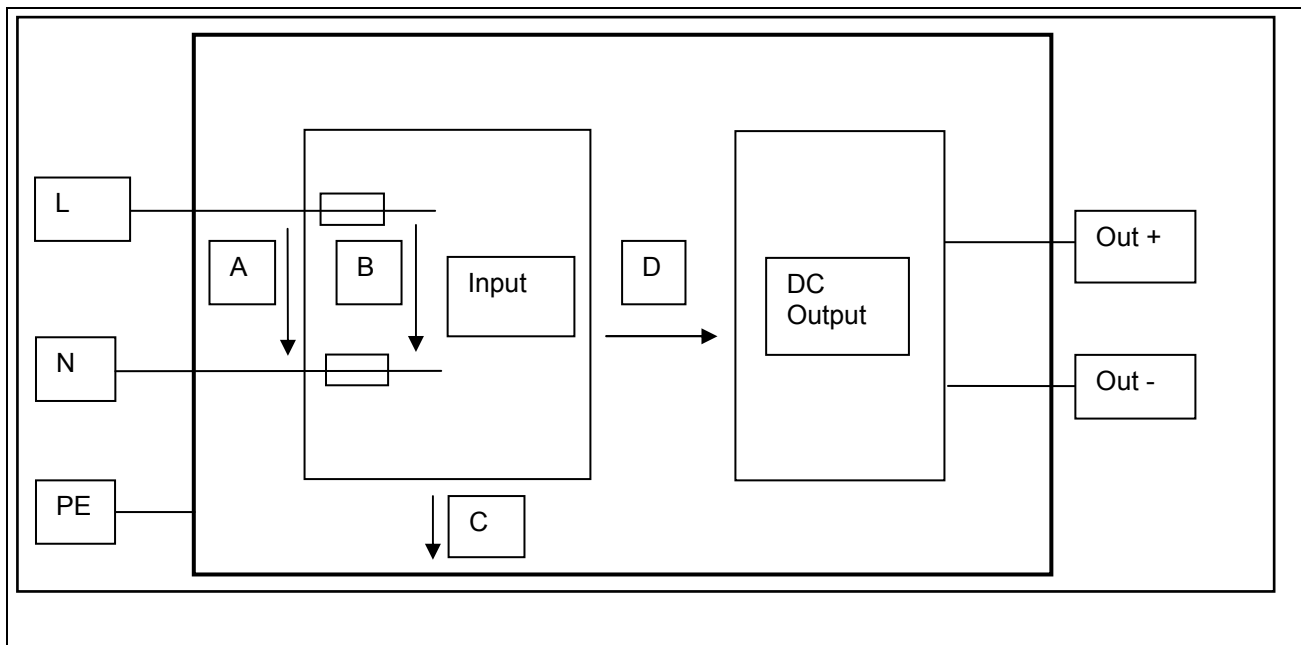

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

TABLE: To insulation diagram									P
Pollution degree : PD 2									—
Overvoltage category : OVC II									—
Altitude : Up to 2.000 meters									—
Additional details on parts considered as applied parts : <input checked="" type="checkbox"/> None <input type="checkbox"/> Areas _____ (See Clause 4.6 for details)									—
Area	Number and type of Means of Protection: MOOP, MOPP	CTI (IIIb, unless is known)	Working voltage		Required creepage (mm)	Required clearance (mm)	Measured creepage (mm)	Measured clearance (mm)	Remarks
Vrms	Vpk								
A	1 x MOPP	IIIb	240	340	2,5	2,0	4,1	4,1	
B	1 x MOPP	IIIb	240	340	Shall be verified via short-circuiting.				
C	1 x MOPP	IIIb	240	340	2,5	5,0	4,3	2,5	
D1	2 x MOPP	IIIb	285	488	6,1	4,2	8,5	8,2	See 1)
D2	2 x MOPP	IIIb	285	488	6,1	4,2	7,1	7,1	See 2)
D3	2 x MOPP	IIIb	265	424	5,5	4,2	6,7	5,3	See 3)

Supplementary information:

- 1) Near transformer T1 on PCB.
- 2) Inside transformer T1.
- 3) Near optocoupler U2, U4.




Clause	Requirement + Test	Result - Remark	Verdict
--------	--------------------	-----------------	---------

Step 4



This is the finished product

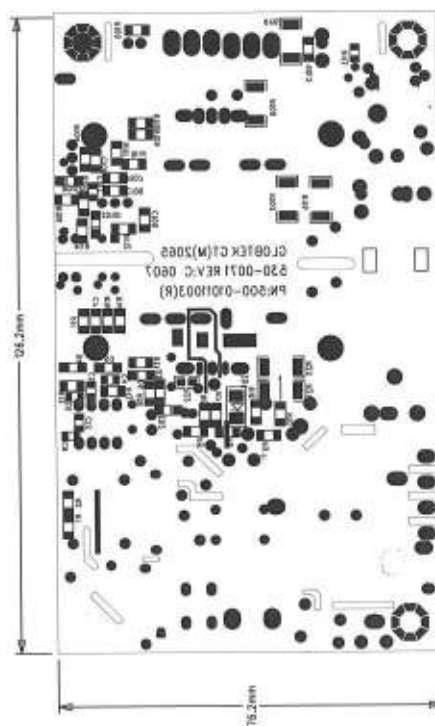

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
4	GENERAL REQUIREMENTS		P
4.1	Requirements of this standard applied in NORMAL USE and reasonably foreseeable misuse	--	P
4.2	A RISK MANAGEMENT PROCESS complying with ISO 14971 was performed	The risk management requirements of the standard were not addressed. The power supply tested in this test report is only component level power supply for building-in.	N/E
4.3	ESSENTIAL PERFORMANCE functions identified according to MANUFACTURER'S policy for RISK acceptability in RISK MANAGEMENT FILE.....	See Appended Table 4.3 and RM Results Table 4.3	N/E
	ESSENTIAL PERFORMANCE functions maintained following particular tests as applicable	Essential performance shall be determined within the end medical equipment; however for this medical power supply intended for building-in essential performance is considered 2 x MOOP (2 x Means of Operator Protection). 2 x MOOP is tested within this test report.	N/E
4.4	EXPECTED SERVICE LIFE stated in RISK MANAGEMENT FILE	Risk management shall be addressed to the end type medical equipment. Expected operating life time specified within safety instructions: 5 years minimum	N/E
4.5	Alternative means of addressing particular RISKS considered acceptable based on MANUFACTURER'S justification that RESIDUAL RISKS resulting from application of alternative means equal to or less than RESIDUAL RISKS resulting from requirements of this standard	See Appended RM Results Table 4.5	N/E
4.6	RISK MANAGEMENT PROCESS identifies parts that can come into contact with PATIENT but not defined as APPLIED PARTS, subjected to the requirements for APPLIED PARTS, except for Clause 7.2.10.....	See Appended Insulation Diagram Table and RM Results Table 4.6 No parts that can come with the patient. EUT is medical power supply unit intended for building-in.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
4.7	ME EQUIPMENT remained SINGLE FAULT SAFE, or the RISK remained acceptable as determined by Clause 4.2	See Appended RM Results Table 4.7 The risk management requirements of the standard were not addressed. All applicable single fault conditions performed according to the standard.	N/E
	Failure of any one component at a time that could result in a HAZARDOUS SITUATION, including those in 13.1, simulated physically or theoretically	See Appended Table 13.2 for simulated physical test, or See Attachment No. __ for theoretical simulation Physically testing performed.	P
	RISK associated with failure of component during EXPECTED SERVICE LIFE of ME EQUIPMENT taken into account to evaluate if a component should be subjected to failure simulation	Short circuit or open circuit of relevant single components performed. See Table 13.2: Single fault conditions in accordance with 13.2.2 to 13.2.13, inclusive.	P
4.8	All components and wiring whose failure could result in a HAZARDOUS SITUATION used according to their applicable ratings, except as specified, or by RISK MANAGEMENT PROCESS.....	See Appended RM Results Table 4.8 (N/E) The risk management requirements of the standard were not addressed. IEC approved components provided within the equipment. See Table 8.10: List of critical components.	P
	Reliability of components used as MEANS OF PROTECTION assessed for conditions of use in ME EQUIPMENT, and they complied with one of the following:	--	P
	a) Applicable safety requirements of a relevant IEC or ISO standard	Approved critical components used. See Table 8.10: List of critical components.	P
	b) Requirements of this standard applied in the absence of a relevant IEC or ISO standard	--	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
4.9	A COMPONENT WITH HIGH-INTEGRITY CHARACTERISTICS provided because a fault in a particular component can generate an unacceptable RISK	See appended Table 8.10 & RM Results Table 4.9 The risk management requirements of the standard were not addressed. Approved components bridging insulation provided within the equipment (optocouplers, bridging capacitors).	N/E
	COMPONENTS WITH HIGH-INTEGRITY CHARACTERISTICS selected and evaluated consistent with their conditions of use and reasonable foreseeable misuse during EXPECTED SERVICE LIFE OF ME EQUIPMENT by reviewing RISK MANAGEMENT FILE	See Appended RM Results Table 4.9 The risk management requirements of the standard were not addressed. Approved components bridging insulation provided within the equipment (optocouplers, bridging capacitors).	N/E
4.10	Power supply		P
4.10.1	ME EQUIPMENT is suitable for connection to a SUPPLY MAINS, specified to be connected to a separate power supply, can be powered by an INTERNAL ELECTRICAL POWER SOURCE, or a combination of the three	Power supply unit intended is suitable for connection to supply mains. Input connector used for connection to the mains. See enclosed pictures of the unit for details.	P
4.10.2	Maximum rated voltage for ME EQUIPMENT intended to be connected to SUPPLY MAINS is 250 V for HAND-HELD ME EQUIPMENT (V)	Not hand-held equipment.	N/A
	– 250 V d.c. or single-phase a.c., or 500 V polyphase a.c. for ME EQUIPMENT and ME SYSTEMS with a RATED input ≤ 4 kVA (V)	Rated input voltage: 100-240 Vac	P
	– 500 V for all other ME EQUIPMENT and ME SYSTEMS	--	N/A
4.11	Power input		P
	Steady-state measured input of ME EQUIPMENT or ME SYSTEM at RATED voltage and at operating settings indicated in instructions for use did not exceed marked rating by more than 10% ..	See appended Table 4.11	P
	– Measurements on ME EQUIPMENT or a ME SYSTEM marked with one or more RATED voltage ranges made at both upper and lower limits of the range	See appended Table 4.11	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Measurements made at a voltage equal to the mean value of the range when each marking of RATED input was related to the mean value of relevant voltage range	--	N/A
	Power input, expressed in volt-amperes, measured with a volt-ampere meter or calculated as the product of steady state current (measured as described above) and supply voltage	See appended Table 4.11 Power input expressed in Amperes. See copy of marking plate for details.	N/A

5	GENERAL REQUIREMENTS FOR TESTING ME EQUIPMENT		P
5.1	TYPE TESTS determined in consideration of Clause 4, in particular 4.2	--	P
	Test not performed when analysis indicated condition being tested was adequately evaluated by other tests or methods	See Appended RM Results Table 5.1 Type test performed according to all applicable clauses of standard IEC 60601-1:2005.	N/A
	Results of RISK ANALYSIS used to determine combination(s) of simultaneous faults to be tested	Applicable single faults performed.	N/E
5.2	TYPE TESTS conducted on one representative sample under investigation; multiple samples used simultaneously when validity of results was not significantly affected	Type test performed on multiple samples. Validity of results not significantly affected.	P
5.3	a) Tests conducted within the environmental conditions specified in technical description	--	P
	Temperature (°C), Relative Humidity (%)	-20 to 50°C temperature (for models without air flow). -20 to 45°C temperature (for models with 10 CFM air flow). 5 to 95% relative humidity	—
	Atmospheric Pressure (kPa)	Atmospheric pressure not influence on the operation of the equipment. EUT is medical power supply unit.	—
	b) ME EQUIPMENT shielded from other influences that might affect the validity of tests	No other influences.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) Test conditions modified and results adjusted accordingly when ambient temperature could not be maintained	Measured temperature rises adjusted to maximum ambient temperature as specified by the manufacturer (maximum ambient temperature specified by the manufacturer: 45°C or 50°C).	P
5.4	a) ME EQUIPMENT tested under least favourable working conditions specified in instructions for use and identified during RISK ANALYSIS, except as noted	See Appended RM Results Table 5.4a Power supply unit is intended for building-in. All test performed in horizontal position 100 mm above the bench. Maximum ambient temperature specified by the manufacturer: 45°C (for models without air flow) or 50°C (for models with 10 CFM air flow). The risk management requirements of the standard were not addressed.	P
	b) ME EQUIPMENT with adjustable or controlled operating values by anyone other than SERVICE PERSONNEL adjusted to values least favourable for the relevant test per instructions for use	No adjustable or controlled operating values provided.	N/A
	c) When test results influenced by inlet pressure and flow or chemical composition of a cooling liquid, tests performed within the limits in technical description	--	N/A
	d) Potable water used for cooling	No provision for cooling provided.	N/A
5.5	Supply voltage during tests was the least favourable of the voltages specified in 4.10 or voltages marked on ME EQUIPMENT (V)	--	P
	ME EQUIPMENT marked with a RATED frequency range tested at the least favourable frequency within the range (Hz)..... :	Supply frequency: 50-60 Hz	P
	ME EQUIPMENT with more than one RATED voltage, or both a.c./ d.c. tested in conditions (see 5.4) related to the least favourable voltage, nature of supply, and type of current..... :	Supply voltage: 100-240 Vac Only AC supply voltage used for supplying power supply unit.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	ME EQUIPMENT tested with alternative ACCESSORIES and components specified in ACCOMPANYING DOCUMENTS to result in the least favourable conditions	Temperature test performed with external air flow as specified by the manufacturer (10 CFM).	P
	ME EQUIPMENT connected to a separate power supply as specified in instructions for use	Mains operated equipment.	N/A
5.6	When failure occurred or probability of future failure detected during sequence of tests, per agreement with manufacturer, all tests affecting results conducted on a new sample	Considered.	P
	Alternatively, upon repair and modification of the sample, only the relevant tests conducted	Considered.	P
5.7	ME EQUIPMENT or parts thereof affected by climatic conditions were set up completely, or partially, with covers detached and subjected to a humidity preconditioning prior to tests of Clauses 8.7.4 and 8.8.3	See Appended RM Results Table 5.7 Complete power supply unit was subject to standard humidity preconditioning treatment (48 hours).	P
	Manually detachable parts removed and treated concurrently with major parts and manually removable ACCESS COVERS were opened and detached	No such parts.	N/A
	ME EQUIPMENT heated to a temperature between T and T + 4 °C for at least 4 h and placed in a humidity chamber with a relative humidity of 93 % ± 3 % and an ambient within 2 °C of T in the range of + 20 °C to + 32 °C for 48 h	Standard humidity treatment performed.	P
	When RISK MANAGEMENT PROCESS indicated ME EQUIPMENT can be exposed to high humidity for extended periods (i.e., out-door use), test time extended proportionally (h).....	See above.	N/A
5.8	Unless stated otherwise, tests in this standard sequenced as in Annex B to prevent results of one test on a subsequent test	Considered.	P
5.9	Determination of APPLIED PARTS and ACCESSIBLE PARTS		N/A
5.9.1	APPLIED PARTS identified by inspection and reference to ACCOMPANYING DOCUMENTS.....	See clause 4.6 Remark No applied parts provided. EUT is medical power supply unit intended for building-in.	N/A
5.9.2	ACCESSIBLE PARTS		N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
5.9.2.1	Accessibility, when necessary, determined using standard test finger of Fig 6 applied in a bent or straight position	See Appended Table 5.9.2 Power supply unit is intended for building-in. It is provided without external enclosure. End product consideration.	N/A
	Openings preventing entry of test finger of Fig. 6 mechanically tested with a straight un-jointed test finger of the same dimensions with a force of 30 N	No external enclosure provided. Power supply unit is intended for building-in.	N/A
	When the straight un-jointed test finger entered, test with the standard test finger (Fig 6) was repeated, if necessary, by pushing the finger through the opening	--	N/A
5.9.2.2	Test hook of Fig. 7 inserted in all openings of ME EQUIPMENT and pulled with a force of 20 N for 10 s	No external enclosure provided. Power supply unit is intended for building-in.	N/A
	All additional parts that became accessible checked using standard test finger and by inspection	--	N/A
5.9.2.3	Conductive parts of actuating mechanisms of electrical controls accessible after removal of handles, knobs, levers and the like regarded as ACCESSIBLE PARTS :	No actuating mechanisms provided. No external enclosure. Power supply unit is intended for building-in.	N/A
	Conductive parts of actuating mechanisms not considered ACCESSIBLE PARTS when removal of handles, knobs, etc. required use of a TOOL, and inspection of RISK MANAGEMENT FILE indicated the relevant part is unlikely to detach unintentionally during EXPECTED SERVICE LIFE OF ME EQUIPMENT.....:	See Appended RM Results Table 5.9.2.3	N/A

6	CLASSIFICATION OF ME EQUIPMENT AND ME SYSTEMS		P
6.2	CLASS I ME EQUIPMENT, externally powered	Power supply unit can be treated as Class I equipment or Class II equipment.	P
	CLASS II ME EQUIPMENT, externally powered	Power supply unit can be treated as Class I equipment or Class II equipment.	P
	INTERNALLY POWERED ME EQUIPMENT	EUT is not internally powered equipment.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	EQUIPMENT with means of connection to a SUPPLY MAINS complied with CLASS I or CLASS II ME EQUIPMENT requirements when so connected, and when not connected to SUPPLY MAINS with INTERNALLY POWERED ME EQUIPMENT requirements	--	N/A
	TYPE B APPLIED PART	No applied parts provided. EUT is medical power supply unit intended for building-in.	N/A
	TYPE BF APPLIED PART	--	N/A
	TYPE CF APPLIED PART	--	N/A
	DEFIBRILLATION-PROOF APPLIED PARTS	--	N/A
6.3	ENCLOSURES classified according to degree of protection against ingress of water and particulate matter (IPN ₁ N ₂) as per IEC 60529	See RM Results Table 11.6.5. Power supply unit is provided without external enclosure.	N/A
6.4	ME EQUIPMENT or its parts intended to be sterilized classified according to method(s) of sterilization in instructions for use	No such parts.	N/A
6.5	ME EQUIPMENT and ME SYSTEMS intended for use in an OXYGEN RICH ENVIRONMENT classified for such use and complied with 11.2.2	EUT was not evaluated for use in an oxygen rich environments.	N/A
6.6	CONTINUOUS or Non-CONTINUOUS OPERATION.....	Power supply unit is designed for continuous operation. No markings provided on the outer side of the enclosure.	P

7	ME EQUIPMENT IDENTIFICATION, MARKING, AND DOCUMENTS		P
7.1.1	RISK of poor USABILITY associated with the design of ME EQUIPMENT'S identification and marking addressed in a USABILITY ENGINEERING PROCESS	See Attachment # EUT is medical power supply unit intended for building-in. Usability not relevant.	N/A
7.1.2	Legibility of Markings Test for Markings specified in Clause 7.2-7.6	See Appended Table 7.1.2 Power supply unit is intended for building-in; therefore legibility of markings not relevant.	N/A
7.1.3	Required markings can be removed only with a TOOL or by appreciable force, are durable and remain CLEARLY LEGIBLE during EXPECTED SERVICE LIFE of ME EQUIPMENT in NORMAL USE	Marking plate with all relevant information provided on the bulk capacitor enclosure.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	a) After tests, adhesive labels didn't loosen up or curl up at edges and markings complied with requirements in Clause 7.1.2..... :	See appended Tables 7.1.3 and 8.10	P
	b) Markings required by 7.2-7.6 remained CLEARLY LEGIBLE after marking durability test ... :	See appended Tables 7.1.3 and 8.10	P
7.2	Marking on the outside of ME EQUIPMENT or ME EQUIPMENT parts		P
7.2.1	At least markings in 7.2.2, 7.2.5, 7.2.6 (not for PERMANENTLY INSTALLED ME EQUIPMENT), 7.2.10, and 7.2.13 were applied when size of EQUIPMENT, its part, an ACCESSORY, or ENCLOSURE did not permit application of all required markings :	See attached copy of Marking Plate All required markings are provided on the marking plate.	P
	Remaining markings fully recorded in ACCOMPANYING DOCUMENTS :	All required markings are provided on the marking plate.	N/A
	Markings applied to individual packaging when impractical to apply to ME EQUIPMENT	Packaging not part of the investigation. EUT is medical power supply unit intended for building-in; therefore individual packaging not safety relevant.	N/A
	A material, component, ACCESSORY, or ME EQUIPMENT intended for a single use, or its packaging marked "Do Not Reuse" or with symbol 28 of Table D.1 (ISO 7000-1051, DB:2004-01)..... :	No such material, component, accessory or equipment parts intended for single use.	N/A
7.2.2	MANUFACTURER's name or trademark marked on ME EQUIPMENT and detachable components..... :	Trademark provided on the marking plate. See copy of marking plate for details.	P
	Misidentification does not present an unacceptable risk	See Appended RM Results Table 7.2.2 The risk management requirements of the standard were not addressed.	N/E
	MODEL OR TYPE REFERENCE also marked, except when misidentification would not present an unacceptable RISK..... :	See attached copy of Marking Plate.	P
	Software forming part of a PEMS identified with a unique identifier, such as revision level or date of release/issue, and identification are available to designated persons :	No software incorporated. EUT is medical power supply unit intended for building-in.	N/A
7.2.3	Symbol 11 on Table D.1 (ISO 7000-1641, DB: 2004-01) used, optionally, advice to OPERATOR to consult ACCOMPANYING DOCUMENTS	Symbol not required. EUT is medical power supply unit intended for building-in.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Safety sign 10 on Table D.2 (safety sign IEC 60878 Safety 01) used, advising OPERATOR that ACCOMPANYING DOCUMENTS must be consulted	--	N/A
7.2.4	ACCESSORIES marked with name or trademark of MANUFACTURER or supplier, and with a MODEL or TYPE REFERENCE	No accessories provided.	N/A
	Markings applied to individual packaging when not practical to apply to ACCESSORIES	--	N/A
7.2.5	MODEL or TYPE REFERENCE of equipment to be connected to ME EQUIPMENT to provide power, is marked adjacent to the relevant connection point when this connection could result in an unacceptable RISK.....	See Appended RM Results Table 7.2.5 EUT is intended for connection to the mains.	N/A
7.2.6	Connection to the Supply Mains		P
	Except for PERMANENTLY INSTALLED ME EQUIPMENT, marking appearing on the outside of part containing SUPPLY MAINS connection and, adjacent to connection point	Marking plate provided on the bulk capacitor enclosure. Power supply unit is intended for building-in.	P
	For PERMANENTLY INSTALLED ME EQUIPMENT, NOMINAL supply voltage or range marked inside or outside of ME EQUIPMENT, preferably, adjacent to supply connection terminals	EUT is not permanently installed equipment.	N/A
	– RATED supply voltage(s) or RATED voltage range(s) with a hyphen (-) between minimum and maximum voltages (V, V-V)	100-240 Vac Markings provided on the marking plate.	P
	Multiple RATED supply voltages or multiple RATED supply voltage ranges are separated by (V/V) ..	--	N/A
	– Nature of supply (e.g., No. of phases, except single-phase) and type of current	Symbol “ ~ ” provided near rated supply voltage.	P
	Symbols 1-5, Table D.1 (symbols of IEC 60417-5032, 5032-1, 5032-2, 5031, and 5033, all DB: 2002-10) used, optionally, for same parameters:	Symbol No. 1 from table D.1 used for input voltage. Symbol No. 4 from table D.1 used for output voltage.	P
	– RATED supply frequency or RATED frequency range in hertz	50-60 Hz	P
	– Symbol 9 of Table D.1 (symbol IEC 60417-5172, DB: 2003-02) used for CLASS II ME EQUIPMENT	Provided on the marking plate of power supply unit.	P
7.2.7	RATED input in amps or volt-amps, or in watts when power factor exceeds 0.9 (A, VA, W)	Rated input expressed in Amperes: 1500-800 mA	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	RATED input for one or more RATED voltage ranges provided for upper and lower limits of the range or ranges when the range(s) is/are greater than $\pm 10\%$ of the mean value of specified range (A, VA,W).....:	Rated input expressed in Amperes: 1500-800 mA	P
	Input at mean value of range marked when range limits do not differ by more than 10 % from mean value (A, VA, W)	--	N/A
	Marking includes long-time and most relevant momentary volt-ampere ratings when provided, each plainly identified and indicated in ACCOMPANYING DOCUMENTS (VA).....:	--	N/A
	Marked input of ME EQUIPMENT provided with means for connection of supply conductors of other electrical equipment includes RATED and marked output of such means (A, VA, W)	--	N/A
7.2.8	Output connectors		P
7.2.8.1	See 16.9.2.1 b) for MULTIPLE SOCKET-OUTLETS integral with ME EQUIPMENT	--	N/A
7.2.8.2	Output connectors are marked, except for MULTIPLE SOCKET-OUTLETS or connectors intended for specified ACCESSORIES or equipment	Rating of the output provided on the marking plate. See copy of marking plate for details.	P
	Rated Voltage (V), Rated Current (A).....:	See copy of marking plate for details.	—
	Rated Power (W), Output Frequency (Hz)	DC output voltage.	—
7.2.9	ME EQUIPMENT or its parts marked with the IP environmental Code per IEC 60529 according to classification in 6.3 (Table D.3, Code 2).....:	Power supply unit is provided without external enclosure; therefore IP protection not relevant.	N/A
7.2.10	Degrees of protection against electric shock as classified in 6.2 for all APPLIED PARTS marked with relevant symbols as follows (not applied to parts identified according to 4.6):	No applied parts provided. EUT is medical power supply unit intended for building-in.	N/A
	TYPE B APPLIED PARTS with symbol 19 of Table D.1 (IEC 60417-5840, DB: 2002-10), not applied in such a way as to give the impression of being inscribed within a square in order to distinguish it from symbol IEC 60417-5333	--	N/A
	TYPE BF APPLIED PARTS with symbol 20 of Table D.1 (IEC 60417-5333, DB: 2002-10)	--	N/A
	TYPE CF APPLIED PARTS with symbol 21 of Table D.1 (IEC 60417-5335, DB: 2002-10)	--	N/A
	DEFIBRILLATION-PROOF APPLIED PARTS marked with symbols 25-27 of Table D.1 (IEC 60417-5841, IEC 60417-5334, or IEC 60417-5336, all DB: 2002-10):	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Proper symbol marked adjacent to or on connector for APPLIED PART, except marked on APPLIED PART when there is no connector, or connector used for more than one APPLIED PART and different APPLIED PARTS with different classifications	--	N/A
	Safety sign 2 of Table D.2 (ISO 7010-W001) placed near relevant outlet when protection against effect of discharge of a cardiac defibrillator is partly in the PATIENT cable	--	N/A
	An explanation indicating protection of ME EQUIPMENT against effects of discharge of a cardiac defibrillator depends on use of proper cables included in instructions for use	--	N/A
7.2.11	ME EQUIPMENT not marked to the contrary assumed to be suitable for CONTINUOUS OPERATION	No markings provided; therefore EUT is intended for continuous operation.	P
	DUTY CYCLE for ME EQUIPMENT intended for non-CONTINUOUS OPERATION appropriately marked to provide maximum "on" and "off" time	EUT is designed for continuous operation.	N/A
7.2.12	Type and full rating of a fuse marked adjacent to ACCESSIBLE fuse-holder	Power supply unit is intended for building-in; therefore primary fuses shall not be accessible by the operator after installation. End product consideration.	N/A
	Fuse type	--	—
	Voltage (V) and Current (A) rating	--	—
	Operating speed (s) and Breaking capacity	--	—
7.2.13	A safety sign CLEARLY LEGIBLE and visible after INSTALLATION in NORMAL USE applied to a prominent location of EQUIPMENT that produce physiological effects capable of causing HARM to PATIENT or OPERATOR not obvious to OPERATOR ..	EUT not produces physiological effects.	N/A
	Nature of HAZARD and precautions for avoiding or minimizing the associated RISK described in instructions for use	See Appended RM Results Table 7.2.13	N/A
7.2.14	HIGH VOLTAGE TERMINAL DEVICES on the outside of ME EQUIPMENT accessible without the use of a TOOL marked with symbol 24 of Table D.1 (symbol IEC 60417-5036, DB: 2002-10)	No such terminals provided.	N/A
7.2.15	Requirements for cooling provisions marked (e.g., supply of water or air)	--	N/A
7.2.16	ME EQUIPMENT with limited mechanical stability	Power supply unit is intended for building-in.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
7.2.17	Packaging marked with special handling instructions for transport and/or storage.....:	EUT is not special handling equipment.	N/A
	Permissible environmental conditions for transport and storage marked on outside of packaging	--	N/A
	Packaging marked with a suitable safety sign indicating premature unpacking of ME EQUIPMENT could result in an unacceptable RISK	See Appended RM Results Table 7.2.17	N/A
	Packaging of sterile ME EQUIPMENT or ACCESSORIES marked sterile	--	N/A
7.2.18	RATED maximum supply pressure from an external source marked on ME EQUIPMENT adjacent to each input connector.....:	No pressure used during normal operation of the power supply unit.	N/A
7.2.19	Symbol 7 of Table D.1 (IEC 60417-5017, DB:2002-10) marked on FUNCTIONAL EARTH TERMINAL.....:	No functional earth terminal provided.	N/A
7.2.20	Protective means, required to be removed to use a particular function of ME EQUIPMENT with alternate applications, marked to indicate the necessity for replacement when the function is no longer needed	--	N/A
	No marking applied when an interlock provided	--	N/A
7.3	Marking on the inside of ME EQUIPMENT or ME EQUIPMENT parts		P
7.3.1	Maximum power loading of heating elements or lamp-holders designed for use with heating lamps marked near or in the heater (W)	No heating elements provided.	N/A
	A marking referring to ACCOMPANYING DOCUMENTS provided for heating elements or lamp-holders designed for heating lamps that can be changed only by SERVICE PERSONNEL using a TOOL	--	N/A
7.3.2	Symbol 24 of Table D.1 (symbol IEC 60417-5036, DB: 2002-10), or safety sign 3 of Table D.2 used to mark presence of HIGH VOLTAGE parts	No such parts within the equipment.	N/A
7.3.3	Type of battery and mode of insertion when applicable is marked	No batteries provided. EUT is intended for connection to the mains.	N/A
	An identifying marking provided referring to instructions in ACCOMPANYING DOCUMENTS for batteries intended to be changed only by SERVICE PERSONNEL using a TOOL	--	N/A
	A warning provided indicating replacement of lithium batteries or fuel cells when incorrect replacement by inadequately trained personnel would result in an unacceptable RISK (e.g., excessive temperatures, fire or explosion).....:	--	N/A
	An identifying marking also provided referring to instructions in ACCOMPANYING DOCUMENTS	See Appended RM Results Table 7.3.3	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
7.3.4	Fuses, replaceable THERMAL CUT-OUTS and OVER-CURRENT RELEASES, accessible by use of a TOOL, marked by type and full rating at the component or by reference to ACCOMPANYING DOCUMENTS	Type and rating of internal non-accessible primary fuses provided near primary fuses: T2,0A 250 V (for 65 W models - models without air flow. T3,15A 250 V (for 80 W models - models with 10 CFM air flow). In additional characteristics provided also within safety instructions.	P
	Type	Characteristics provided within safety instructions.	—
	Voltage (V) and Current (A) rating.....	Characteristics provided within safety instructions.	—
	Operating speed (s) and Breaking capacity.....	Characteristics provided within safety instructions.	—
7.3.5	PROTECTIVE EARTH TERMINAL marked with symbol 6 of Table D.1 (IEC 60417-5019, DB: 2002-10), except for the PROTECTIVE EARTH TERMINAL in an APPLIANCE INLET according to IEC 60320-1	Correct symbol provided near protective earth terminal (Symbol 6 of Table D.1).	P
	Markings on or adjacent to PROTECTIVE EARTH TERMINALS not applied to parts requiring removal to make the connection, and remained visible after connection made	--	P
7.3.6	Symbol 7 of Table D.1 (IEC 60417-5017, DB: 2002 -10) marked on FUNCTIONAL EARTH TERMINALS	No functional earth terminal provided.	N/A
7.3.7	Terminals for supply conductors marked adjacent to terminals, except when no HAZARD would result when interchanging connections	See Appended RM Results Table 7.3.7 Power supply unit is intended for building-in and provided with input connector for connection to the mains (CON 1).	N/A
	Terminal markings included in ACCOMPANYING DOCUMENTS when ME EQUIPMENT too small to accommodate markings	--	N/A
	Terminals exclusively for neutral supply conductor in PERMANENTLY INSTALLED ME EQUIPMENT marked with Code 1 of Table D.3 (Code in IEC 60445)	--	N/A
	Marking for connection to a 3-phase supply, if necessary, complies with IEC 60445	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Markings on or adjacent to electrical connection points not applied to parts requiring removal to make connection, and remained visible after connection made	--	N/A
7.3.8	“For supply connections, use wiring materials suitable for at least X °C” (where X > than max temperature measured in terminal box or wiring compartment under NORMAL USE), or equivalent, marked at the point of supply connections	--	N/A
	Statement not applied to parts requiring removal to make the connection, and CLEARLY LEGIBLE after connections made	--	N/A
7.4	Marking of controls and instruments		N/A
7.4.1	The “on” & “off” positions of switch to control power to ME EQUIPMENT or its parts, including mains switch, marked with symbols 12 and 13 of Table D.1 (IEC 60417-5007, DB: 2002-10, and IEC 60417-5008, DB: 2002-10), or	No mains switch provided. EUT is medical power supply unit intended for building-in.	N/A
	– indicated by an adjacent indicator light, or	--	N/A
	– indicated by other unambiguous means	--	N/A
	The “on/off” positions of push button switch with bi-stable positions marked with symbol 14 of Table D.1 (IEC 60417-5010 DB: 2002-10), and	--	N/A
	– status indicated by adjacent indicator light	--	N/A
	– status indicated by other unambiguous means	--	N/A
	The “on/off” positions of push button switch with momentary on position marked with symbol 15 of Table D.1 (symbol 60417-5011 DB: 2002-10), or	--	N/A
	– status indicated by adjacent indicator light	--	N/A
	– status indicated by other unambiguous means	--	N/A
7.4.2	Different positions of control devices/switches indicated by figures, letters, or other visual means	No control devices provided.	N/A
	Controls provided with an associated indicating device when change of setting of a control could result in an unacceptable RISK to PATIENT in NORMAL USE, or	See Appended RM Results Table 7.4.2	N/A
	– an indication of direction in which magnitude of the function changes	--	N/A
7.4.3	Numeric indications of parameters on ME EQUIPMENT expressed in SI units according to ISO 31 except the base quantities listed in Table 1 expressed in the indicated units	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	ISO 1000 applied for application of SI units, their multiples, and certain other units	--	N/A
	All Markings in Sub-clause 7.4 complied with tests and criteria of 7.1.2 and 7.1.3	See Appended Tables 7.1.2 and 7.1.3.	N/A
7.5	Safety signs		N/A
	Markings used to convey a warning, prohibition or mandatory action mitigating a RISK not obvious to OPERATOR are safety signs from ISO 7010	See Appended RM Results Table 7.5 No safety signs provided. EUT is medical power supply unit intended for building-in.	N/A
	Affirmative statement together with safety sign placed in instructions for use if insufficient space on ME EQUIPMENT	--	N/A
	Specified colours in ISO 3864-1 used for safety signs.....:	--	N/A
	Safety notices include appropriate precautions or instructions on how to reduce RISK(s)	--	N/A
	Safety signs including any supplementary text or symbols described in instructions for use	--	N/A
7.6	Symbols		P
7.6.1	Meanings of symbols used for marking described in instructions for use	Provided within user instruction.	P
7.6.2	Symbols required by this standard conform to IEC or ISO publication referenced	According to Annex D.	P
7.6.3	Symbols used for controls and performance conform to the IEC or ISO publication where symbols are defined, as applicable	--	N/A
7.7	Colours of the insulation of conductors		P
7.7.1	PROTECTIVE EARTH CONDUCTOR identified by green and yellow insulation	Internal PE conductor with green/yellow insulation. See enclosed pictures of the unit for details.	P
7.7.2	Insulation on conductors inside ME EQUIPMENT forming PROTECTIVE EARTH CONNECTIONS identified by green and yellow at least at terminations	Internal PE conductor with green/yellow insulation.	P
7.7.3	Green and yellow insulation identify only following conductors:	--	P
	– PROTECTIVE EARTH CONDUCTORS	--	P
	– conductors specified in 7.7.2	--	N/A
	– POTENTIAL EQUALIZATION CONDUCTORS	No potential equalization provided.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– FUNCTIONAL EARTH CONDUCTORS	No functional earth provided.	N/A
7.7.4	Neutral conductors of POWER SUPPLY CORDS are “light blue” specified in IEC 60227-1 or IEC 60245-1	No power supply cord provided. EUT is medical power supply unit intended for building-in.	N/A
7.7.5	Colours of conductors in POWER SUPPLY CORDS in accordance with IEC 60227-1 or IEC 60245-1	--	N/A
7.8	Indicator lights and controls		P
7.8.1	Red indicator lights mean: Warning (i.e., immediate response by OPERATOR required)	No red indicator lights provided.	N/A
	Yellow indicator lights mean: Caution (i.e., prompt response by OPERATOR required)	No yellow indicator lights provided.	N/A
	Green indicator lights mean: Ready for use	Green indicator light provided to indicate power “ON”.	P
	Other colours, if used: Meaning other than red, yellow, or green (colour, meaning)..... :	No other indicator lights provided.	N/A
7.8.2	Red used only for emergency control	--	N/A
7.9	ACCOMPANYING DOCUMENTS		P
7.9.1	ME EQUIPMENT accompanied by documents containing at least instructions for use, and a technical description	Technical specifications provided by the manufacturer. EUT is medical power supply unit intended therefore user manual as required for end medical product not relevant.	P
	ACCOMPANYING DOCUMENTS identify ME EQUIPMENT by the following, as applicable:	--	P
	– Name or trade-name of MANUFACTURER and an address the RESPONSIBLE ORGANIZATION can be referred to	GLOBTEK with address provided within technical specifications.	P
	– MODEL OR TYPE REFERENCE	Model name provided within technical specifications.	P
	When ACCOMPANYING DOCUMENTS provided electronically (e.g., on CDROM), RISK MANAGEMENT PROCESS includes instructions as to what is required in hard copy or as markings on ME EQUIPMENT (for emergency operation)	See Appended RM Results Table 7.9.1 Paper version provided.	N/A
	ACCOMPANYING DOCUMENTS specify special skills, training, and knowledge required of OPERATOR or RESPONSIBLE ORGANIZATION and environmental restrictions on locations of use	Power supply unit is intended for building-in.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	ACCOMPANYING DOCUMENTS written at a level consistent with education, training, and other needs of individuals for whom they are intended	Power supply unit is intended for building-in.	P
7.9.2	Instructions for use include the required information		P
7.9.2.1	– intended use of ME EQUIPMENT,	EUT is medical power supply unit intended for building-in. It is intended for supplying end medical product by its output voltage (output connector provided).	P
	– frequently used functions, and	EUT is medical power supply unit intended for building-in. It is intended for supplying end medical product by its output voltage (output connector provided).	P
	– known contraindication(s) to use of ME EQUIPMENT	EUT is medical power supply unit; therefore no contraindications to use of the equipment.	N/A
	Classifications as in Clause 6, all markings per Clause 7.2, and explanation of safety signs and symbols marked on ME EQUIPMENT	Provided within technical specifications.	P
	Instructions for use are in a language acceptable to the intended operator	Only English version evaluated.	P
7.9.2.2	Instructions for use include all warning and safety notices	Provided within technical specifications.	P
	Warning statement for CLASS I ME EQUIPMENT indicating: “WARNING: To avoid risk of electric shock, this equipment must only be connected to a supply mains with protective earth”	Provided within safety instructions.	P
	Warnings regarding significant RISKS of reciprocal interference posed by ME EQUIPMENT during specific investigations or treatments	--	N/A
	Information on potential electromagnetic or other interference and advice on how to avoid or minimize such interference	Not specified. EUT is medical power supply unit intended for building-in. Shall be evaluated during end medical product approval.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Warning statement for ME EQUIPMENT supplied with an integral MULTIPLE SOCKET-OUTLET indicating, "connecting electrical equipment to MSO effectively leads to creating an ME SYSTEM, and can result in a reduced level of safety"	--	N/A
	The RESPONSIBLE ORGANIZATION is referred to this standard for the requirements applicable to ME SYSTEMS	--	N/A
7.9.2.3	Statement on ME EQUIPMENT for connection to a separate power supply indicating "power supply is specified as a part of ME EQUIPMENT or combination is specified as a ME SYSTEM"	EUT is intended for connection to the mains.	N/A
7.9.2.4	Warning statement for mains- operated ME EQUIPMENT with additional power source not automatically maintained in a fully usable condition indicating the necessity for periodic checking or replacement of power source	No additional power source provided. EUT is intended for connection to the mains.	N/A
	Warning to remove primary batteries when ME EQUIPMENT is not likely to be used for some time when leakage from battery would result in an unacceptable RISK..... :	See Appended RM Results Table 7.9.2.4	N/A
	Specifications of replaceable INTERNAL ELECTRICAL POWER SOURCE when provided	--	N/A
	Warning indicating ME EQUIPMENT must be connected to an appropriate power source when loss of power source would result in an unacceptable RISK..... :	See Appended RM Results Table 7.9.2.4	N/A
7.9.2.5	Instructions for use include a description of ME EQUIPMENT, its functions, significant physical and performance characteristics together with the expected positions of OPERATOR, PATIENT, or other persons near ME EQUIPMENT in NORMAL USE	Provided within user instructions.	P
	Information provided on materials and ingredients PATIENT or OPERATOR is exposed to when such exposure can constitute an unacceptable RISK	--	N/A
	Restrictions specified on other equipment or NETWORK/DATA COUPLINGS, other than those forming part of an ME SYSTEM, to which a SIGNAL INPUT/OUTPUT PART may be connected	--	N/A
	APPLIED PARTS specified	No applied parts provided. EUT is medical power supply unit intended for building-in.	N/A
7.9.2.6	Information provided indicating where the installation instructions may be found or information on qualified personnel who can perform the installation	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
7.9.2.7	Instructions provided indicating not to position ME EQUIPMENT to make it difficult to operate the disconnection device when an APPLIANCE COUPLER or separable plug is used as isolation means to meet 8.11.1 a)	Shall be provided within user manual of the end medical product. EUT is medical power supply unit intended for building-in.	N/A
7.9.2.8	Necessary information provided for OPERATOR to bring ME EQUIPMENT into operation including initial control settings, and connection to or positioning of PATIENT prior to use of ME EQUIPMENT, its parts, or ACCESSORIES	--	N/A
7.9.2.9	Information provided to operate ME EQUIPMENT including explanation of controls, displays and signals, sequence of operation, connection of detachable parts or ACCESSORIES, replacement of material consumed during operation	--	N/A
	Meanings of figures, symbols, warning statements, abbreviations and indicator lights described in instructions for use	--	N/A
7.9.2.10	A list of all system messages, error messages, and fault messages provided with an explanation of messages including important causes and possible action(s) to be taken to resolve the problem indicated by the message	Not messages provided.	N/A
7.9.2.11	Information provided for the OPERATOR to safely terminate operation of ME EQUIPMENT	End product consideration. Power supply unit is intended for building-in. Green indicator light provided to indicate "ON" operation of the power supply unit.	N/A
7.9.2.12	Information provided on cleaning, disinfection, and sterilization methods, and applicable parameters that can be tolerated by ME EQUIPMENT parts or ACCESSORIES specified	No applied parts provided. EUT is medical power supply unit intended for building-in.	N/A
	Components, ACCESSORIES or ME EQUIPMENT marked for single use, except when required by MANUFACTURER to be cleaned, disinfected, or sterilized prior to use	No such parts.	N/A
7.9.2.13	Instructions provided on preventive inspection, calibration, maintenance and its frequency	EUT is maintenance free. No preventive inspection, calibration and maintenance necessary.	N/A
	Information provided for safe performance of routine maintenance necessary to ensure continued safe use of ME EQUIPMENT	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Parts requiring preventive inspection and maintenance to be performed by SERVICE PERSONNEL identified including periods of application	No such parts specified by the manufacturer.	N/A
	Instructions provided to ensure adequate maintenance of ME EQUIPMENT containing rechargeable batteries to be maintained by anyone other than SERVICE PERSONNEL	No rechargeable batteries incorporated. EUT is intended for connection to the mains.	N/A
7.9.2.14	A list of ACCESSORIES, detachable parts, and materials for use with ME EQUIPMENT provided	--	N/A
	Other equipment providing power to ME SYSTEM sufficiently described (e.g. part number, RATED VOLTAGE, max or min power, protection class, intermittent or continuous service)	EUT is intended for connection to the mains.	N/A
7.9.2.15	RISKS associated with disposal of waste products, residues, etc., and of ME EQUIPMENT and ACCESSORIES at the end of their EXPECTED SERVICE LIFE are identified, and instructions provided on minimizing these RISKS :	Provided within user instructions: The power supply has to be disposed appropriately. Please refer to local regulations (Waste Electrical and Electronic Equipment).	P
7.9.2.16	Instructions for use include information specified in 7.9.3 or identify where it can be found (e.g. in a service manual)	--	N/A
7.9.3	Technical description		P
7.9.3.1	All essential data provided for safe operation, transport, storage, and measures or conditions necessary for installing ME EQUIPMENT, and preparing it for use including the following:	--	P
	– information as in clause 7.2	Technical specifications and safety instructions provided by the manufacturer.	P
	– permissible environmental conditions of use including conditions for transport and storage	Operating conditions specified within safety instructions. -0 to 45°C temperature (for models without air flow) -0 to 50°C temperature (for models with 10 CFM air flow). 5 to 90% relative humidity Storage conditions specified within safety instructions: -40°C to 80°C temperature 5 to 90% humidity	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– all characteristics of ME EQUIPMENT including range(s), accuracy, and precision of displayed values or where they can be found	--	N/A
	– special installation requirements such as max. permissible apparent impedance of SUPPLY MAINS	Not specified by the manufacturer.	N/A
	– permissible range of values of inlet pressure and flow, and chemical composition of cooling liquid used for cooling	--	N/A
	– a description of means of isolating ME EQUIPMENT from SUPPLY MAINS, when such means not in ME EQUIPMENT	Power supply unit is intended for building-in. End product consideration.	N/A
	– a description of means for checking oil level in partially sealed oil filled ME EQUIPMENT or its parts when applicable	--	N/A
	– a warning statement addressing HAZARDS that can result from unauthorized modification of ME EQUIPMENT according to following examples	--	P
	“WARNING: No modification of this equipment is allowed”	Provided within safety instructions.	P
	“WARNING: Do not modify this equipment without authorization of the manufacturer”	--	N/A
	“WARNING: If this equipment is modified, appropriate inspection and testing must be conducted to ensure continued safe use of equipment”	--	N/A
	Technical description separable from instructions for use contains required information, as follows		N/A
	– information as in clause 7.2	EUT is medical power supply unit intended for building-in. Technical specifications and safety instructions provided by the manufacturer.	N/A
	– all applicable classifications in Clause 6, warning and safety notices, and explanation of safety signs marked on ME EQUIPMENT	--	N/A
	– a brief description of ME EQUIPMENT, how it functions, and its significant physical and performance characteristics	--	N/A
	MANUFACTURER’S optional requirements for minimum qualifications of SERVICE PERSONNEL documented in technical description	--	N/A
7.9.3.2	The technical description contains the following required information		P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	–type and full rating of fuses used in SUPPLY MAINS external to PERMANENTLY INSTALLED ME EQUIPMENT, when type and rating of fuses are not apparent from information on RATED current and mode of operation of ME EQUIPMENT :	See Appended RM Results Table 7.9.3.2 EUT is not permanently installed equipment.	N/A
	– a statement for ME EQUIPMENT with a non-DETACHABLE POWER SUPPLY CORD if POWER SUPPLY CORD is replaceable by SERVICE PERSONNEL, and if so, instructions for correct connection and anchoring to ensure compliance with 8.11.3	No power supply cord provided. EUT is provided with input connector for connection to the mains.	N/A
	– instructions for correct replacement of interchangeable or detachable parts specified by MANUFACTURER as replaceable by SERVICE PERSONNEL, and	No such parts within the equipment.	N/A
	– warnings identifying nature of HAZARD when replacement of a component could result in an unacceptable RISK, and when replaceable by SERVICE PERSONNEL all information necessary to safely replace the component	There is a note within the safety instructions related to the service personnel: Please use only components approved by the manufacturer.	P
7.9.3.3	Technical description indicates, MANUFACTURER will provide circuit diagrams, component part lists, descriptions, calibration instructions to assist to SERVICE PERSONNEL in parts repair	--	N/A
7.9.3.4	Means used to comply with requirements of 8.11.1 clearly identified in technical description	Power supply unit is intended for building-in. End product consideration.	N/A

8	PROTECTION AGAINST ELECTRICAL HAZARDS FROM ME EQUIPMENT		P
8.1	Limits specified in Clause 8.4 not exceeded for ACCESSIBLE PARTS and APPLIED PARTS in NORMAL or SINGLE FAULT CONDITIONS	--	P
	NORMAL CONDITION considered as simultaneous occurrence of situations identified in 8.1a)	--	P
	SINGLE FAULT CONDITION considered to include the occurrences as specified in Clause 8.1b)... :	See Appended RM Results Tables 8.1b(1), (2), (3)	N/A
	ACCESSIBLE PARTS determined according to 5.9	EUT is medical power supply unit intended for building-in without external enclosure. End product consideration.	N/A
	LEAKAGE CURRENTS measured according to 8.7	--	P
8.2	Requirements related to power sources		N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.2.1	When ME EQUIPMENT specified for connection to a separate power source other than SUPPLY MAINS, separate power source considered as part of ME EQUIPMENT or combination considered as an ME SYSTEM	EUT is intended for connection to the mains.	N/A
	Tests performed with ME EQUIPMENT connected to separate power supply when one specified	--	N/A
	When a generic separate power supply specified, specification in ACCOMPANYING DOCUMENTS examined	--	N/A
8.2.2	No HAZARDOUS SITUATION other than absence of ESSENTIAL PERFORMANCE developed when a connection with wrong polarity made for ME EQUIPMENT from an external d.c. source	See Appended RM Results Table 8.2.2 EUT is intended for connection to the mains.	N/A
	ME EQUIPMENT connected with correct polarity did not present an unacceptable RISK	--	N/A
	Protective devices that can be reset by anyone without a TOOL restore correct operation on reset	--	N/A
8.3	Classification of APPLIED PARTS		N/A
	a) APPLIED PART specified in ACCOMPANYING DOCUMENTS as suitable for DIRECT CARDIAC APPLICATION IS TYPE CF	No applied parts provided. EUT is medical power supply unit intended for building-in.	N/A
	b) An APPLIED PART provided with a PATIENT CONNECTION intended to deliver electrical energy or an electrophysiological signal to or from PATIENT IS TYPE BF OR CF APPLIED PART	--	N/A
	c) An APPLIED PART not covered by a) or b) is a TYPE B, BF, OR CF	--	N/A
	d) Requirements of a TYPE B APPLIED PART applied to a part in 4.6 to be subjected to requirements for an APPLIED PART (except marking)	--	N/A
	Requirements for a TYPE BF or CF APPLIED PART applied as in RISK MANAGEMENT PROCESS	See Appended RM Results Table 8.3d	N/A
8.4	Limitation of voltage, current or energy		P
8.4.1	PATIENT CONNECTIONS intended to deliver Current		N/A
	Limits in 8.4.2 not applied to currents intended to flow through body of PATIENT to produce a physiological effect during NORMAL USE	No patient connections.	N/A
8.4.2	ACCESSIBLE PARTS including APPLIED PARTS		P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	a) Currents from, to, or between PATIENT CONNECTIONS did not exceed limits for PATIENT LEAKAGE CURRENT and PATIENT AUXILIARY CURRENT per Tables 3 and 4 when measured according to Clause 8.7.4..... :	See appended Table 8.7 No applied parts.	N/A
	b) LEAKAGE CURRENTS from, to, or between ACCESSIBLE PARTS did not exceed limits for TOUCH CURRENT in Cl. 8.7.3 c) when measured per Clause 8.7.4 (mA) :	See appended Table 8.7 Power supply unit is intended for building-in without external enclosure. Touch current measured on the output connector only for reference. Shall be evaluated during end medical product approval.	P
	c) Limits specified in b) not applied to parts when probability of a connection to a PATIENT, directly or through body of OPERATOR, is negligible in NORMAL USE, and the OPERATOR is appropriately instructed	See Appended RM Results Table 8.4.2c	N/A
	– accessible contacts of connectors	--	N/A
	– contacts of fuseholders accessible during replacement of fuse	--	N/A
	– contacts of lampholders accessible after removal of lamp	--	N/A
	– parts inside an ACCESS COVER that can be opened without a TOOL, or where a TOOL is needed but the instructions for use instruct an OPERATOR other than SERVICE PERSONNEL to open the relevant ACCESS COVER	--	N/A
	Voltage to earth or to other ACCESSIBLE PARTS did not exceed 42.4 V peak a.c. or 60 V d.c. for above parts in NORMAL or single fault condition (V a.c. or d.c.) :	See appended Table 8.4.2 Measured on the output.	P
	Limit of 60 V d.c applied with no more than 10% peak-to-peak ripple, and when ripple larger than specified value, 42.4 V peak limit applied (V d.c.) :	See appended Table 8.4.2 Measured on the output.	P
	Energy did not exceed 240 VA for longer than 60 s or stored energy available did not exceed 20 J at a potential up to 2 V (VA or J) :	See appended Table 8.4.2 Measured on the output.	P
	LEAKAGE CURRENT limits referred to in 8.4.2 b) applied when voltages higher than limits in 8.4.2 c) were present (mA) :	See appended Table 8.4.2	N/A
	d) Voltage and energy limits specified in c) above also applied to the following:	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– internal parts, other than contacts of plugs, connectors and socket-outlets, touchable by test pin in Fig 8 inserted through an opening in an ENCLOSURE; and	--	N/A
	– internal parts touchable by a metal test rod with a diameter of 4 mm and a length of 100 mm, inserted through any opening on top of ENCLOSURE or through any opening provided for adjustment of pre-set controls using a TOOL	No such parts.	N/A
	Test pin or the test rod inserted through relevant openings with minimal force of no more than 1 N	Power supply unit is intended for building-in without external enclosure.	N/A
	Test rod inserted in every possible position through openings provided for adjustment of pre-set controls that can be adjusted in NORMAL USE, with a force of 10 N	--	N/A
	Test repeated with a TOOL specified in instructions for use	--	N/A
	Test rod freely and vertically suspended through openings on top of ENCLOSURE	--	N/A
	e) Devices used to de-energize parts when an ACCESS COVER opened without a TOOL gives access to parts at voltages above levels permitted by this Clause comply with 8.11.1 for mains isolating switches and remain effective in SINGLE FAULT CONDITION	--	N/A
	A TOOL is required when it is possible to prevent the devices from operating	--	N/A
8.4.3	Worst case voltage between pins of plug and between either supply pin and ENCLOSURE did not exceed 60 V one s after disconnecting the plug of ME EQUIPMENT or its parts (V) :	See appended Table 8.4.3	P
	A triggering circuit used to ensure disconnection occurred at peak of supply voltage waveform	--	P
	When voltage exceeded 60 V, calculated or measured stored charge didn't exceed 45 μ C ... :	See appended Table 8.4.3	N/A
8.4.4	Residual voltage of conductive parts of capacitive circuits, having become accessible after ME EQUIPMENT was de-energized after removal of ACCESS COVERS, didn't exceed 60V or calculated stored charge didn't exceed 45 μ C... :	See appended Table 8.4.4	N/A
	A device manually discharging capacitors used when automatic discharging was not possible and ACCESS COVERS could be removed only with aid of a TOOL	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Capacitor(s) and connected circuitry marked with symbol 24 of Table D.1 (IEC 60417-5036, DB: 2002-10), and manual discharging device specified in technical description..... :	--	N/A
8.5	Separation of parts		P
8.5.1	MEANS OF PROTECTION (MOP)		P
8.5.1.1	Two MEANS OF PROTECTION provided for ME EQUIPMENT to prevent APPLIED and other ACCESSIBLE PARTS from exceeding limits in 8.4	2 x MOOP provided between primary secondary circuit and 1 x MOOP between primary circuit and protective earth within the equipment.	P
	Each MEANS OF PROTECTION categorized as a MEANS OF PATIENT PROTECTION or a MEANS OF OPERATOR PROTECTION, taking into account Clause 4.6, and flow chart in Fig A.12	Protection categorized as operator protection.	P
	Varnishing, enameling, oxidation, and similar protective finishes and coatings with sealing compounds replasticizing at temperatures expected during operation and sterilization disregarded as MEANS OF PROTECTION	--	N/A
	Coatings and other insulation intended as a MEANS OF PROTECTION complying with IEC 60950-1:2001 considered acceptable as a MEANS OF OPERATOR PROTECTION but not automatically as a MEANS OF PATIENT PROTECTION	Considered.	P
	RISK MANAGEMENT PROCESS taken into consideration for MEANS OF PATIENT PROTECTION	No applied parts provided. EUT is medical power supply unit intended for building-in.	N/A
	Components and wiring forming a MEANS OF PROTECTION comply with 8.10	See list of critical components for details.	P
	Insulation, CREEPAGE, CLEARANCES, components or earth connections not complying with 8.5.1.2 and 8.5.1.3 not considered as MEANS OF PROTECTION, and failure of these parts regarded as NORMAL CONDITION	Considered.	P
8.5.1.2	MEANS OF PATIENT PROTECTION (MOPP)	Protection categorized as operator protection.	N/A
	Solid insulation forming a MEANS OF PATIENT PROTECTION complied with dielectric strength test of Clause 8.8 at test voltage of Table 6	--	N/A
	CREEPAGE and CLEARANCES forming a MEANS OF PATIENT PROTECTION complied with Table 12	--	N/A
	PROTECTIVE EARTH CONNECTIONS forming a MEANS OF PATIENT PROTECTION complied with Cl. 8.6	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	A Y1 capacitor complying with IEC 60384-14 and having passed dielectric strength test for two MEANS OF PATIENT PROTECTION considered equivalent to one MEANS OF PATIENT PROTECTION	See Appended Tables 8.8.3 and 8.10	N/A
	Two capacitors used in series, each RATED for total WORKING VOLTAGE across the pair and have the same NOMINAL capacitance	--	N/A
	Voltage Total Working (V) and C Nominal (μF)..... :	--	—
8.5.1.3	MEANS OF OPERATOR PROTECTION (MOOP)	Protection categorized as operator protection.	P
	Solid insulation forming a MEANS OF OPERATOR PROTECTION complied with:	--	N/A
	– dielectric strength test of 8.8 at test voltage of Table 6; or	--	P
	– requirements of IEC 60950-1 for INSULATION CO-ORDINATION	--	N/A
	CREEPAGE and CLEARANCES forming a MEANS OF OPERATOR PROTECTION complied with:	--	P
	– limits of Tables 13 to 16 (inclusive); or	--	P
	– requirements of IEC 60950-1 for INSULATION CO-ORDINATION	--	N/A
	PROTECTIVE EARTH CONNECTIONS forming a MEANS OF OPERATOR PROTECTION complied with Cl. 8.6, or	--	P
	– requirements and tests of IEC 60950-1 for protective earthing..... :	See Attachment #	N/A
	A Y2 capacitor complying with IEC 60384-14 and passing dielectric strength test for one MEANS OF OPERATOR PROTECTION considered equivalent to one MEANS OF OPERATOR PROTECTION	See Appended Tables 8.8.3 and 8.10 Y2 capacitors provided between primary circuit and protective earth (CY7, CY8, CY1 and CY2).	P
	A Y1 capacitor complying with IEC 60384-14 and having passed dielectric strength test for two MEANS OF OPERATOR PROTECTION considered equivalent to two MEANS OF OPERATOR PROTECTION	See Appended Tables 8.8.3 and 8.10 Y1 capacitors provided between primary and secondary circuit (CY3, CY4).	P
	Two capacitors used in series each RATED for total WORKING VOLTAGE across the pair and have the same NOMINAL capacitance	Single capacitors provided.	N/A
	Voltage Total Working (V) and C Nominal (μF)..... :	--	—

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Points at which impedances of components, CREEPAGE, CLEARANCES, PROTECTIVE EARTH CONNECTIONS or insulation, prevent ACCESSIBLE PARTS from exceeding limits in 8.4 examined whether a failure at any of these points is to be regarded as a NORMAL or SINGLE FAULT CONDITION	--	N/A
	A MEANS OF PROTECTION protecting APPLIED PARTS, or parts identified by 4.6 as parts subject to the same requirements, considered MEANS OF PATIENT PROTECTION..... :	--	N/A
	A MEANS OF PROTECTION protecting other parts considered MEANS OF OPERATOR PROTECTION :	Considered.	P
8.5.2	Separation of PATIENT CONNECTIONS		N/A
8.5.2.1	PATIENT CONNECTIONS of F-TYPE APPLIED PART separated from all other parts by equivalent to one MEANS OF PATIENT PROTECTION for a WORKING VOLTAGE equal to maximum MAINS VOLTAGE and complied with limit for PATIENT LEAKAGE CURRENT at 110 % of max. MAINS VOLTAGE :	See appended Table 8.7. No applied parts provided. No patient connections provided.	N/A
	Separation requirement not applied between multiple functions of a single F-TYPE APPLIED PART	--	N/A
	PATIENT CONNECTIONS treated as one APPLIED PART in the absence of electrical separation between PATIENT CONNECTIONS of same or another function	--	N/A
	MANUFACTURER has defined if multiple functions are to be considered as all within one APPLIED PART or as multiple APPLIED PARTS :	--	N/A
	Classification as TYPE BF, CF, or DEFIBRILLATION-PROOF applied to one entire APPLIED PART	--	N/A
	LEAKAGE CURRENT tests conducted per 8.7.4 :	See appended Table 8.7	N/A
	Dielectric strength test conducted per 8.8.3.... :	See appended Table 8.8.3	N/A
	CREEPAGE and CLEARANCES measured per 8.9 and Tables 11 to 16 as applicable	--	N/A
	A protective device connected between PATIENT CONNECTIONS of an F-TYPE APPLIED PART and ENCLOSURE to protect against excessive voltages did not operate below 500 V r.m.s	--	N/A
8.5.2.2	PATIENT CONNECTIONS of a TYPE B APPLIED PART not PROTECTIVELY EARTHED are separated by one MEANS OF PATIENT PROTECTION from metal ACCESSIBLE PARTS not PROTECTIVELY EARTHED :	See Appended RM Results Table 8.5.2.2	N/A
	– except when metal ACCESSIBLE PART is physically close to APPLIED PART and can be regarded as a part of APPLIED PART; and	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– RISK that metal ACCESSIBLE PART will make contact with a source of voltage or LEAKAGE CURRENT above permitted limits is acceptably low	--	N/A
	LEAKAGE CURRENT tests conducted per 8.7.4:	See appended Table 8.7	N/A
	Dielectric strength test conducted per 8.8.3:	See appended Table 8.8.3	N/A
	Relevant CREEPAGE and CLEARANCES measured per 8.9 and Tables 11 to 16 as applicable	--	N/A
	The RISK MANAGEMENT FILE reviewed	--	N/A
8.5.2.3	A connector on a PATIENT lead located at the end of the lead remote from PATIENT, with conductive part not separated from all PATIENT CONNECTIONS by one MEANS OF PATIENT PROTECTION for a WORKING VOLTAGE equal to MAXIMUM MAINS VOLTAGE		N/A
	- cannot be connected to earth or hazardous voltage while the PATIENT CONNECTIONS are in contact with PATIENT.....:	See Appended RM Results Table 8.5.2.3 No patient leads provided.	N/A
	– conductive part of connector not separated from all PATIENT CONNECTIONS did not come into contact with a flat conductive plate of not less than 100 mm diameter	--	N/A
	– CLEARANCE between connector pins and a flat surface is at least 0.5 mm	--	N/A
	– conductive part pluggable into a mains socket protected from making contact with parts at MAINS VOLTAGE by insulation with a CREEPAGE DISTANCE of at least 1.0 mm, a 1500 V dielectric strength and complying with 8.8.4.1	--	N/A
	– required test finger did not make electrical contact with conductive part when applied against access openings with a force of 10 N, except when RISK MANAGEMENT PROCESS indicated no unacceptable RISK existed from contact with objects other than a mains socket or a flat surface	See Appended RM Results Table 8.5.2.3	N/A
8.5.3	MAXIMUM MAINS VOLTAGE		P
	– MAXIMUM MAINS VOLTAGE determined to be the highest RATED supply voltage for single-phase or d.c. SUPPLY MAINS powered ME EQUIPMENT, as well as INTERNALLY POWERED ME EQUIPMENT with a means of connection to a SUPPLY MAINS (V)	Supply voltage: 100-240 Vac	P
	When less than 100 V, MAXIMUM MAINS VOLTAGE was 250 V	--	N/A
	– MAXIMUM MAINS VOLTAGE was the highest RATED phase to neutral supply voltage for poly-phase ME EQUIPMENT (V)	Single-phase equipment.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– for other INTERNALLY POWERED ME EQUIPMENT, maximum mains voltage was 250 V	Not internally powered equipment. EUT is intended for connection to the mains.	N/A
8.5.4	WORKING VOLTAGE	--	P
	– Input supply voltage to ME EQUIPMENT was RATED voltage or voltage within RATED range resulting in highest measured value (V) :	Supply voltage: 100-240 Vac Working voltage measurements performed at 240 Vac and with rated output load.	P
	– WORKING VOLTAGE for d.c. voltages with superimposed ripple was average value when peak-to-peak ripple less than 10% of average value or peak voltage when peak-to-peak ripple exceeding 10% of average value (V)..... :	--	N/A
	– WORKING VOLTAGE for each MEANS OF PROTECTION forming DOUBLE INSULATION was voltage DOUBLE INSULATION, as a whole, subjected to (V)..... :	See Insulation Diagram and Insulation Table.	P
	– Intentional or accidental earthing of PATIENT regarded as a NORMAL CONDITION for WORKING VOLTAGE involving a PATIENT CONNECTION not connected to earth	--	N/A
	– WORKING VOLTAGE between PATIENT CONNECTIONS of an F-TYPE APPLIED PART and ENCLOSURE was highest voltage appearing across insulation in NORMAL USE including earthing of any part of APPLIED PART (V)..... :	No applied parts provided.	N/A
	– WORKING VOLTAGE for DEFIBRILLATION-PROOF APPLIED PARTS determined disregarding possible presence of defibrillation voltages	No applied parts provided.	N/A
	– WORKING VOLTAGE was equal to resonance voltage in case of motors provided with capacitors between the point where a winding and a capacitor are connected together and a terminal for external conductors (V)..... :	No motors provided.	N/A
8.5.5	DEFIBRILLATION-PROOF APPLIED PARTS	No applied parts provided.	N/A
8.5.5.1	Classification “DEFIBRILLATION-PROOF APPLIED PART” applied to one APPLIED PART in its entirety, but not separate functions of same APPLIED PART	--	N/A
	Possibility of an OPERATOR receiving a shock from such parts taken into consideration in RISK MANAGEMENT PROCESS	--	N/A
	Isolation of PATIENT CONNECTIONS of a DEFIBRILLATION-PROOF APPLIED PART from other parts of ME EQUIPMENT accomplished as follows:	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	a) No hazardous electrical energies appear during a discharge of cardiac defibrillator	See Appended Table 8.5.5.1a	N/A
	b) ME EQUIPMENT complied with relevant requirements of this standard, providing BASIC SAFETY and ESSENTIAL PERFORMANCE following exposure to defibrillation voltage, and recovery time stated in ACCOMPANYING DOCUMENTS	See Appended Table 8.5.5.1b	N/A
8.5.5.2	Means provided to limit energy delivered to a 100 Ω load to at least 90% of energy delivered to this load with ME EQUIPMENT disconnected ...	See Appended Table 8.5.5.2	N/A
8.6	Protective and functional earthing and potential equalization of ME EQUIPMENT		P
8.6.1	Requirements of 8.6.2 to 8.6.8 applied	--	P
	Parts complying with IEC 60950-1 for protective earthing and serving as MEANS OF OPERATOR PROTECTION but not PATIENT PROTECTION exempted from requirements of 8.6.2 to 8.6.8	--	N/A
8.6.2	PROTECTIVE EARTH TERMINAL is suitable for connection to an external protective earthing system by a PROTECTIVE EARTH CONDUCTOR in a POWER SUPPLY CORD and a suitable plug or by a FIXED PROTECTIVE EARTH CONDUCTOR	PE terminal provided near supply connector. See enclosed pictures of the unit for details.	P
	Clamping means of PROTECTIVE EARTH TERMINAL of ME EQUIPMENT for FIXED supply conductors or POWER SUPPLY CORDS comply with 8.11.4.3, and cannot be loosened without TOOL	No clamping means provided. See enclosed pictures of the unit for details.	N/A
	Screws for internal PROTECTIVE EARTH CONNECTIONS completely covered or protected against accidental loosening from outside.....	--	N/A
	Earth pin of APPLIANCE INLET forming supply connection to ME EQUIPMENT regarded as PROTECTIVE EARTH TERMINAL	No appliance inlet provided.	N/A
	PROTECTIVE EARTH TERMINAL not used for mechanical connection between different parts of ME EQUIPMENT or securing components not related to protective or functional earthing	Not used for other purposes.	N/A
8.6.3	PROTECTIVE EARTH CONNECTION not used for a moving part, except when MANUFACTURER demonstrated in RISK MANAGEMENT FILE connection will remain reliable during EXPECTED SERVICE LIFE	See Appended RM Results Table 8.6.3 No moving parts provided.	N/A
8.6.4	a) PROTECTIVE EARTH CONNECTIONS carried fault currents reliably and without excessive voltage drop	See appended Table 8.6.4 Test performed with 25 A and 40 A for UL (Canada).	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	b) Allowable TOUCH CURRENT and PATIENT LEAKAGE CURRENT in SINGLE FAULT CONDITION were not exceeded, when impedance of PROTECTIVE EARTH CONNECTIONS exceeded values in 8.6.4 a) and Table 8.6.4, due to limited current capability of relevant circuits :	See appended Table 8.6.4 & Clause 8.7	N/A
8.6.5	Surface coatings		N/A
	Poorly conducting surface coatings on conductive elements removed at the point of contact	--	N/A
	Coating not removed when requirements for impedance and current-carrying capacity met	--	N/A
8.6.6	Plugs and sockets		N/A
	PROTECTIVE EARTH CONNECTION where connection between SUPPLY MAINS and ME EQUIPMENT or between separate parts of ME EQUIPMENT made via a plug and socket was made before and interrupted after supply connections	--	N/A
	- applied also where interchangeable parts are PROTECTIVELY EARTHED	--	N/A
8.6.7	Terminal for connection of a POTENTIAL EQUALIZATION CONDUCTOR		N/A
	– Terminal is accessible to OPERATOR with ME EQUIPMENT in any position of NORMAL USE	No potential equalization conductor provided.	N/A
	– RISK of accidental disconnection minimized in NORMAL USE	--	N/A
	– Terminal allows conductor to be detached without a TOOL	--	N/A
	– Terminal not used for a PROTECTIVE EARTH CONNECTION	--	N/A
	– Terminal marked with symbol 8 of Table D.1 (i.e., symbol IEC 60417-5021)	--	N/A
	– Instructions for use contain information on function and use of POTENTIAL EQUALIZATION CONDUCTOR together with a reference to requirements of this standard	--	N/A
	POWER SUPPLY CORD does not incorporate a POTENTIAL EQUALIZATION CONDUCTOR	--	N/A
8.6.8	FUNCTIONAL EARTH TERMINAL not used to provide a PROTECTIVE EARTH CONNECTION	--	N/A
8.6.9	Class II ME EQUIPMENT		N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Third conductor of POWER SUPPLY CORD connected to protective earth contact of MAINS PLUG provided with CLASS II ME EQUIPMENT with isolated internal screens used as functional earth connection to the screen's FUNCTIONAL EARTH TERMINAL, coloured green and yellow	--	N/A
	Two MEANS OF PROTECTION provided by insulation of internal screens and all internal wiring connected to them with a related explanation in technical description..... :	--	N/A
8.7	LEAKAGE CURRENTS and PATIENT AUXILIARY CURRENTS		P
8.7.1	a) Electrical isolation providing protection against electric shock limits currents to values in 8.7.3 :	See appended Tables 8.7	P
	b) Specified values of EARTH LEAKAGE, TOUCH, PATIENT LEAKAGE, and PATIENT AUXILIARY CURRENTS applied in combination of conditions in appended Table 8.7 :	See appended Tables 8.7	P
8.7.2	Allowable values specified in 8.7.3 applied under SINGLE FAULT CONDITIONS of 8.1 b), except	--	P
	– where insulation used in conjunction with a PROTECTIVE EARTH CONNECTION, insulation short circuited only under conditions in 8.6.4 b)	--	N/A
	– the only SINGLE FAULT CONDITION for EARTH LEAKAGE CURRENT was interruption of one supply conductor at a time	Considered.	P
	– LEAKAGE CURRENTS and PATIENT AUXILIARY CURRENT not measured in SINGLE FAULT CONDITION of short circuiting of one constituent part of DOUBLE INSULATION	Considered.	P
	SINGLE FAULT CONDITIONS not applied at same time as special test conditions of MAXIMUM MAINS VOLTAGE on APPLIED PARTS and non-PROTECTIVELY EARTHED parts of ENCLOSURE	No applied parts provided.	N/A
8.7.3	Allowable Values		P
	a) Allowable values in 8.7.3 b), c), and d) measured based on, and are relative to currents in Fig 12 a), or by a device measuring frequency contents of currents as in Fig 12 b) :	See appended Table 8.7 Leakage current meter with frequency characteristics as specified on Fig. 12 b) used.	P
	b) Allowable values of PATIENT LEAKAGE and AUXILIARY CURRENTS are according to Tables 3 & 4, and values of a.c. are relative to currents having a frequency not less than 0.1Hz :	See appended Table 8.7 No applied parts provided.	N/A
	c) TOUCH CURRENT did not exceed 100 μ A in NORMAL CONDITION and 500 μ A in SINGLE FAULT CONDITION (I_{TNC} , I_{TSFC}) :	See appended Table 8.7	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	d) EARTH LEAKAGE CURRENT did not exceed 5 mA in NORMAL CONDITION and 10 mA in SINGLE FAULT CONDITION (I_{ENC} , I_{ESFC})	See appended Table 8.7	P
	Higher values of EARTH LEAKAGE CURRENT permitted for PERMANENTLY INSTALLED ME EQUIPMENT connected to a supply circuit supplying only this ME EQUIPMENT according to local regulations or IEC 60364-7-710	See appended Table 8.7 EUT not permanently installed equipment.	N/A
	e) LEAKAGE CURRENTS, regardless of waveform and frequency, did not exceed 10 mA r.m.s. in NORMAL or in SINGLE FAULT CONDITION (measured with a non-frequency-weighted device)	See appended Table 8.7	N/A
8.7.4	LEAKAGE and PATIENT AUXILIARY CURRENTS measurements	See appended Table 8.7	P
8.8	Insulation		P
8.8.1	Insulation relied on as MEANS OF PROTECTION, including REINFORCED INSULATION and insulation between parts of opposite polarity of MAINS PART on SUPPLY MAINS side of mains fuse or OVER-CURRENT RELEASE	--	P
	Insulation exempted from test (complies with clause 4.8)	--	N/A
	Insulation forming MEANS OF OPERATOR PROTECTION and complying with IEC 60950-1 for INSULATION CO-ORDINATION not tested as in 8.8	--	N/A
8.8.2	Distance through solid insulation or use of thin sheet material		P
	Solid insulation forming SUPPLEMENTARY or REINFORCED INSULATION for a PEAK WORKING VOLTAGE greater than 71 V provided with:	--	P
	a) 0.4 mm, min, distance through insulation, or	Optocoupler (See enclosed certificate).	P
	b) does not form part of an ENCLOSURE and not subject to handling or abrasion during NORMAL USE, and comprised of:	--	P
	– at least two layers of material, each passed the appropriate dielectric strength test, or	See appended Table 8.8.3	N/A
	– three layers of material, for which all combinations of two layers together passed the appropriate dielectric strength test	See appended Table 8.8.3 Approved triple insulated wire used for secondary windings within the transformer.	P
	Dielectric strength test for one or two layers was same as for one MEANS OF PROTECTION for SUPPLEMENTARY INSULATION	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Dielectric strength test for one or two layers was same as for two MEANS OF PROTECTION for REINFORCED INSULATION	Approved triple insulated wire used for secondary windings within the transformer.	N/A
	BASIC, SUPPLEMENTARY, and REINFORCED INSULATION required between windings of wound components separated by interleaved insulation complying with a) or b), or both, except when	--	P
	c) Wire with solid insulation, other than solvent based enamel, complying with a)	--	N/A
	d) Wire with multi-layer extruded or spirally wrapped insulation complying with b) and complying with Annex L	Approved triple insulated wire used for secondary according to Annex U of IEC/EN 60950-1 (the same requirements as within Annex L of IEC/EN 60601-1).	P
	e) Finished wire with spirally wrapped or multi-layer extruded insulation, complying with Annex L	--	N/A
	– BASIC INSULATION: minimum two wrapped layers or one extruded layer	--	N/A
	– SUPPLEMENTARY INSULATION: minimum two layers, wrapped or extruded	--	N/A
	– REINFORCED INSULATION: minimum three layers, wrapped or extruded	--	N/A
	In d) and e), for spirally wrapped insulation with CREEPAGE DISTANCES between layers less than in Table 12 or 16 (Pollution Degree 1) depending on type of insulation, path between layers sealed as a cemented joint in 8.9.3.3 and test voltages of TYPE TESTS in L.3 equal 1.6 times of normal values	--	N/A
	Protection against mechanical stress provided where two insulated wires or one bare and one insulated wire are in contact inside wound component, crossing at an angle between 45° and 90° and subject to winding tension	--	N/A
	Finished component complied with routine dielectric strength tests of 8.8.3.....:	See appended Table 8.8.3	N/A
	Tests of Annex L not repeated since material data sheets confirm compliance	See Table 8.10 and Material Information Attachment	N/A
8.8.3	Dielectric Strength		P
	Solid insulating materials with a safety function withstood dielectric strength test voltages	See appended Table 8.8.3	P
8.8.4	Insulation other than wire insulation		P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.8.4.1	Resistance to heat retained by all insulation and insulating partition walls during EXPECTED SERVICE LIFE OF ME EQUIPMENT	--	P
	ME EQUIPMENT and RISK MANAGEMENT FILE examined in conjunction with resistance to moisture, dielectric strength, and mechanical strength tests	See Appended RM Results Table 8.8.4.1 The risk management requirements of the standard were not addressed.	N/E
	Satisfactory evidence of compliance provided by manufacturer for resistance to heat	Manufacturer is using approved materials with adequate temperature characteristics. See Table 8.10: List of critical components for details.	P
	Tests conducted in absence of satisfactory evidence for resistance to heat	--	N/A
	a) ENCLOSURE and other external parts of insulating material, except insulation of flexible cords and parts of ceramic material, subjected to ball-pressure test using apparatus of Fig 21	See Table 8.8.4.1	N/A
	b) Parts of insulating material supporting uninsulated parts of MAINS PART subjected to ball-pressure test in a), except at $125^{\circ}\text{C} \pm 2^{\circ}\text{C}$ or ambient indicated in technical description $\pm 2^{\circ}\text{C}$ plus temperature rise determined during test of 11.1 of relevant part, if higher ($^{\circ}\text{C}$)	See Table 8.8.4.1	N/A
	Test not performed on parts of ceramic material, insulating parts of commutators, brush-caps, and similar, and on coil formers not used as REINFORCED INSULATION	--	N/A
8.8.4.2	Resistance to environmental stress		P
	Insulating characteristics and mechanical strength of all MEANS OF PROTECTION not likely to be impaired by environmental stresses including deposition of dirt resulting from wear of parts within EQUIPMENT, potentially reducing CREEPAGE and CLEARANCES below 8.9	Approved material used for insulation.	P
	Ceramic and similar materials not tightly sintered, and beads alone not used as SUPPLEMENTARY OR REINFORCED INSULATION	No such materials used for insulation.	N/A
	Insulating material with embedded heating conductors considered as one MEANS OF PROTECTION but not two MEANS OF PROTECTION	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Parts of natural latex rubber aged by suspending samples freely in an oxygen cylinder containing commercial oxygen to a pressure of 2.1 MPa \pm 70 kPa, with an effective capacity of at least 10 times volume of samples	Rubber not used for insulation.	N/A
	There were no cracks visible to naked eyes after samples kept in cylinder at 70 °C \pm 2 °C for 96h, and afterwards, left at room temperature for at least 16h	--	N/A
8.9	CREEPAGE DISTANCES and AIR CLEARANCES		P
8.9.1.1	CREEPAGE DISTANCES and AIR CLEARANCES are \geq to values in Tables 11 to 16 (inclusive), except as specified in Clauses 8.9.1.2 to 8.9.1.15	--	P
8.9.1.2	Tables 11 to 16 (inclusive) not applied to CREEPAGE and CLEARANCES forming MEANS OF OPERATOR PROTECTION per IEC 60950-1 for INSULATION CO-ORDINATION and used under conditions compliance was tested	--	N/A
8.9.1.3	Specified min CLEARANCE applied as min CREEPAGE for CREEPAGE DISTANCES across glass, mica, ceramic and other inorganic insulating materials with similar tracking characteristics	No such insulation material provided.	N/A
8.9.1.4	When min CREEPAGE derived from Tables 11 to 16 (inclusive) was less than min applicable CLEARANCE, value of min CLEARANCE applied as min CREEPAGE DISTANCE	Considered.	P
8.9.1.5	ME EQUIPMENT RATED to operate at an altitude of 2000 m	EUT was evaluated for use up to 2.000 meters.	P
	ME EQUIPMENT RATED to operate at an altitude specified by MANUFACTURER (m) :	--	N/A
	Operating altitude corresponding to actual air pressure for ME EQUIPMENT intended for pressurized environments (e.g., aircraft) used to determine multiplication factor from Table 8, and AIR CLEARANCE was multiplied by this factor	--	N/A
	CREEPAGE DISTANCES not subjected to multiplication factors, but were at least as large as the resulting value for AIR CLEARANCE	--	N/A
8.9.1.6	When WORKING VOLTAGE was between those in Tables 11 to 16 (inclusive), CREEPAGE and CLEARANCES calculated as follows:	--	P
	– CREEPAGE DISTANCES determined by linear interpolation between the nearest two values, and the calculated spacing rounded off to the next higher 0.1 mm increment (mm) :	See Insulation Diagram/Table. Considered.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– CLEARANCES for PEAK WORKING VOLTAGES above 2800 V peak or d.c. determined by linear interpolation between the nearest two values, and the calculated spacing rounded off to the next higher 0.1 mm increment (mm)..... :	See Insulation Diagram/Table. No such voltages obtained during normal use of the equipment.	N/A
	– for AIR CLEARANCES corresponding to PEAK WORKING VOLTAGE up to 2800 V peak or d.c., the higher of the two values applied	No such voltages obtained during normal use of the equipment.	N/A
8.9.1.7	Material groups classified in accordance with Table 9 (Material Group)..... :	See Insulation Diagram/Table.	P
	Material group evaluated using 50 drops of solution A based on test data for material according to IEC 60112	See attached test data	N/A
	Material of unknown group considered IIIb	--	P
8.9.1.8	– Pollution degree 1: Micro-environment sealed to exclude dust and moisture	--	N/A
	– Pollution degree 2: Micro-environment with non-conductive pollution, except occasional conductivity caused by condensation	EUT was evaluated for use within pollution degree 2 environmental.	P
	– Pollution degree 3: Micro-environment subject to conductive pollution, or dry non-conductive pollution that could become conductive due to expected condensation	--	N/A
	– Pollution degree 4: Micro-environment where continuous conductivity occurs due to conductive dust, rain, or other wet conditions	--	N/A
	Pollution degree 4 not used for insulation providing a MEANS OF PROTECTION	--	N/A
	Where insulation between MAINS PART and earth might be compromised, measures such as maintenance ensure that micro-environment is mitigated to a lower pollution degree	--	N/A
8.9.1.9	Overvoltage category classification; value of MAINS TRANSIENT VOLTAGE determined from overvoltage category per IEC60664-1 and NOMINAL a.c. MAINS VOLTAGE using Table 10	--	P
	V_{MT} Peak (V)	2.500	—
	V_{MN} r.m.s (V)	300	—
8.9.1.10	AIR CLEARANCE for MAINS PARTS (operating on RATED MAINS VOLTAGES up to 300 V) were values for r.m.s. or d.c. RATED MAINS VOLTAGE in Table 13 plus additional CLEARANCE in Table 14 for PEAK WORKING VOLTAGE	Considered.	P
8.9.1.11	SUPPLY MAINS overvoltage category II applied according to IEC 60664-1	--	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	For ME EQUIPMENT intended for overvoltage category III, Tables 13 to 15 (inclusive) not used for clearance, instead values in the next MAINS TRANSIENT VOLTAGE column upwards used	--	N/A
	When PATIENT protection (Table 12) is required for use of ME EQUIPMENT on overvoltage category III SUPPLY MAINS, guidance provided on values required in the rationale for Cl. 8.9 used	No applied parts provided.	N/A
8.9.1.12	A SECONDARY CIRCUIT derived from a SUPPLY MAINS, normally, considered to be overvoltage category I according to IEC 60664-1 when the MAINS PART is overvoltage category II (Table 15)	--	N/A
	Table 15 applied to earthed SECONDARY CIRCUIT or INTERNALLY POWERED ME EQUIPMENT	--	N/A
	Requirements for primary circuits in Tables 13 and 14 used for an unearthed SECONDARY CIRCUIT derived from a SUPPLY MAINS	--	N/A
	Table 15 applied when SECONDARY CIRCUIT was separated from MAINS PART by a functionally earthed or PROTECTIVELY EARTHED metal screen or transients in SECONDARY CIRCUIT were below the levels expected for overvoltage category I	--	N/A
	Table 15 column for circuits not subject to transient overvoltages applied to:	--	N/A
	– d.c. SECONDARY CIRCUITS reliably connected to earth and have capacitive filtering limiting peak-to-peak ripple to 10 % of d.c. voltage, and	--	N/A
	– circuits in INTERNALLY POWERED ME EQUIPMENT	EUT is not internally powered equipment.	N/A
8.9.1.13	For PEAK WORKING VOLTAGES above 1400 V peak or d.c. Table 15 not applied since all the following conditions were met:	No such voltages under normal use of the equipment.	N/A
	– CLEARANCE was at least 5 mm	--	N/A
	– insulation complied with dielectric strength test of 8.8.3 using an a.c. test voltage with an r.m.s. value equal to 1.06 times PEAK WORKING VOLTAGE, or	--	N/A
	– a d.c. test voltage equal to peak value of a.c. test voltage with an r.m.s. value equal to 1.06 times PEAK WORKING VOLTAGE, and	--	N/A
	– CLEARANCE path was partly or entirely through air or along the surface of an insulating material of material group I	--	N/A
	Dielectric strength test conducted only across part(s) of the path that are through air when CLEARANCE path was also partly along surface of a non- group I material	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.9.1.14	Minimum CREEPAGE DISTANCES for two MEANS OF OPERATOR PROTECTION obtained by doubling values in Table 16 for one MEANS OF OPERATOR PROTECTION	Considered.	P
8.9.1.15	CREEPAGE DISTANCES and AIR CLEARANCES for DEFIBRILLATION-PROOF APPLIED PARTS are 4 mm or more to meet 8.5.5.1	No applied parts provided.	N/A
8.9.2	a) Short circuiting of each single one of CREEPAGE DISTANCES and CLEARANCES in turn did not result in a HAZARDOUS SITUATION for insulation in MAINS PART between parts of opposite polarity, therefore, min CREEPAGE and CLEARANCES not applied..... :	See appended Table 8.9.2 Sufficient creepage and clearance distances provided between parts of opposite polarity before mains fuses. Short circuit performed after primary fuses. No hazardous situation.	N/A
	b) Contribution to CREEPAGE DISTANCES of grooves or air gaps less than 1 mm wide limited to widths	Considered.	P
	c) Relative positioning of CLEARANCE providing a MEANS OF PROTECTION is such that the relevant parts are rigid and located by molding, or there is no reduction of a distance below specified value by deformation or movement of parts	--	P
	Normal or likely limited movements of relevant parts taken into consideration when calculating minimum AIR CLEARANCE	--	N/A
8.9.3	Spaces filled by insulating compound		P
8.9.3.1	Only solid insulation requirements applied where distances between conductive parts filled with insulating compound were such that CLEARANCES and CREEPAGE DISTANCES don't exist	Thermal cycling performed during separately approval of incorporated optocoupler (See enclosed certificate).	P
	Thermal cycling, humidity preconditioning, and dielectric strength tests in 8.9.3.2 and 8.9.3.4 or 8.9.3.3 and 8.9.3.4 conducted	--	N/A
8.9.3.2	For insulating compound forming solid insulation between conductive parts, a single sample subjected to thermal cycling PROCEDURE of 8.9.3.4 followed by humidity preconditioning per 5.7 (for 48 hours), followed by dielectric strength test (clause 8.8.3), test voltage multiplied by 1.6..... :	See appended Table 8.9.3.2	N/A
	Cracks or voids in insulating compound affecting homogeneity of material didn't occur	--	N/A
8.9.3.3	Where insulating compound forms a cemented joint with other insulating parts, three samples tested for reliability of joint	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	A winding of solvent-based enamelled wire replaced for the test by a metal foil or by a few turns of bare wire placed close to cemented joint, and three samples tested as follows:	--	N/A
	– One sample subjected to thermal cycling PROCEDURE of 8.9.3.4, and immediately after the last period at highest temperature during thermal cycling, it was subjected to dielectric strength test of 8.8.3 except at 1.6 times the test voltage	See appended Table 8.9.3.4	N/A
	– The other two samples subjected to humidity preconditioning of 5.7, except for 48 hours only followed by a dielectric strength test of 8.8.3 at 1.6 times the test voltage	--	N/A
8.9.3.4	One sample containing the cemented joint subjected to a sequence of temperature cycling tests for 10 times	See appended Table 8.9.3.4	N/A
8.10	Components and wiring		P
8.10.1	Components of ME EQUIPMENT likely to result in an unacceptable RISK by their movements mounted securely as indicated in RISK MANAGEMENT FILE	See Appended RM Results Table 8.10.1 All components mounted securely. Glue used for fixing some components. See enclosed pictures of the unit for details.	N/A
8.10.2	Conductors and connectors of ME EQUIPMENT adequately secured or insulated to prevent accidental detachment in a HAZARDOUS SITUATION	See Appended RM Results Table 8.10.2 Only PE conductor provided (through the hole method in addition to soldering).	P
	Conductors and connectors of ME EQUIPMENT when breaking free at their joint are not capable of touching circuit points resulting in a HAZARDOUS SITUATION as indicated in RISK MANAGEMENT FILE	--	P
	Breaking free of one means of mechanical restraint considered a SINGLE FAULT CONDITION	Considered.	P
	Stranded conductors are not solder-coated when secured by clamping means to prevent HAZARDOUS SITUATIONS due to poor contact	--	N/A
8.10.3	Flexible cords detachable without a TOOL used to interconnect different parts of ME EQUIPMENT provided with means for connection to comply with requirements for metal ACCESSIBLE PARTS of 8.4 when a connection is loosened or broken as shown by measurement or using test finger	See Appended Table 5.9.2 No such flexible cords provided.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.10.4	Cord-connected HAND-HELD parts and cord-connected foot-operated control devices		N/A
8.10.4.1	Control devices of ME EQUIPMENT and their connection cords contain only conductors and components operating at 42.4 V peak a.c., max, or 60 V d.c. in circuits isolated from MAINS PART by two MEANS OF PROTECTION	EUT is not cord-connected hand-held parts and cord-connected foot-operated control devices.	N/A
	d.c. limit of 60 V applied to d.c. with no more than 10 % peak-to-peak ripple	--	N/A
	42.4 V peak limit applied when ripple exceeded 10 % peak-to-peak limit	--	N/A
8.10.4.2	Connection and anchorage of a flexible cord to a HAND-HELD or foot-operated control device of ME EQUIPMENT at both ends of cable to control device complied with 8.11.3 when breaking free or shorting between conductors could result in a HAZARDOUS SITUATION	--	N/A
	This requirement applied to other HAND-HELD parts when disturbance or breaking of one or more of connections could result in a HAZARDOUS SITUATION	--	N/A
8.10.5	Mechanical protection of wiring		N/A
	a) Internal cables and wiring adequately protected against contact with a moving part or from friction at sharp corners and edges where damage to insulation could result in a HAZARDOUS SITUATION	See Appended RM Results Table 8.10.5 No moving parts provided.	N/A
	b) Wiring, cord forms, or components are not likely to be damaged during assembly or during opening or closing of ACCESS COVERS where such damage could result in a HAZARDOUS SITUATION as shown by manual tests and RISK MANAGEMENT FILE	--	N/A
8.10.6	Guiding rollers of insulated conductors prevent bending of movable insulated conductors around a radius of less than five times the outer diameter of the lead concerned in NORMAL USE	--	N/A
8.10.7	a) Insulating sleeve that can only be removed by breaking or cutting, or secured at both ends, is used on internal wiring of when needed	See appended Table 8.10 No insulation sleeve used.	N/A
	b) Sheath of a flexible cord not used as a MEANS OF PROTECTION inside ME EQUIPMENT when it is subject to mechanical or thermal stresses beyond its RATED characteristics	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) Insulated conductors subject to temperatures > 70 °C in NORMAL USE provided with insulation of heat-resistant material when compliance is likely to be impaired due to deterioration of insulation.....:	See appended Table 8.10 No such high temperature rises obtained during normal use of the equipment.	N/A
8.11	MAINS PARTS, components and layout		P
8.11.1	a) ME EQUIPMENT provided with means of electrically isolating its circuits from SUPPLY MAINS simultaneously on all poles.....:	See appended Table 8.10 EUT is intended for building-in; therefore disconnecting device is end product consideration.	N/A
	PERMANENTLY INSTALLED ME EQUIPMENT connected to a poly-phase SUPPLY MAINS equipped with a device not interrupting neutral conductor, provided local installation conditions prevent voltage on neutral conductor from exceeding limits in 8.4.2 c)	EUT is not permanently installed equipment.	N/A
	b) Means of isolation incorporated in ME EQUIPMENT, and external means described in technical description	See appended Table 8.10 End product consideration.	N/A
	c) A SUPPLY MAINS switch used to comply with 8.11.1 a) complies with CREEPAGE and CLEARANCES in IEC 61058-1 for a MAINS TRANSIENT VOLTAGE of 4 kV	See appended Table 8.10	N/A
	d) A SUPPLY MAINS switch not incorporated in a POWER SUPPLY CORD or external flexible lead	--	N/A
	e) Direction of movement of actuator of a SUPPLY MAINS switch used to comply with 8.11.1 a) complies with IEC 60447	--	N/A
	f) A suitable plug device such as an APPLIANCE COUPLER or a flexible cord with a MAINS PLUG used in non-PERMANENTLY INSTALLED ME EQUIPMENT to isolate it from SUPPLY MAINS considered to comply with 8.11.1 a)	See appended Table 8.10 End product consideration.	N/A
	g) A fuse or a semiconductor device not used as an isolating means	--	N/A
	h) ME EQUIPMENT not provided with a device causing disconnection of ME EQUIPMENT from SUPPLY MAINS by producing a short circuit resulting in operation of an overcurrent protection device	End product consideration.	N/A
	i) Parts within ENCLOSURE of ME EQUIPMENT with a circuit > 42.4 V peak a.c. or 60 V d.c. that cannot be disconnected from its supply by an external switch or a plug device accessible at all times is protected against touch even after opening ENCLOSURE by an additional covering	No such parts.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	A clear warning notice is marked on outside of ME EQUIPMENT to indicate it exceeds allowable touch voltage (symbol 10 of Table D.1 is insufficient)	--	N/A
	For a part that could not be disconnected from supply by an external switch or a plug device accessible at all times, the required cover or warning notice complied with this clause	--	N/A
	Standard test finger of Fig 6 applied	--	N/A
8.11.2	MULTIPLE SOCKET-OUTLETS integral with ME EQUIPMENT complied with 16.2 d), second dash; and 16.9.2	No multiple-socket outlet provided.	N/A
8.11.3	POWER SUPPLY CORDS		N/A
8.11.3.1	MAINS PLUG not fitted with more than one POWER SUPPLY CORD	No power supply cord provided. EUT is intended for building-in.	N/A
8.11.3.2	POWER SUPPLY CORDS are no less robust than ordinary tough rubber sheathed flexible cord (IEC 60245-1:2003, Annex A, designation 53) or ordinary polyvinyl chloride sheathed flexible cord (IEC 60227-1:1993, Annex A, design. 53).. :	See appended Table 8.10	N/A
	Only polyvinyl chloride insulated POWER SUPPLY CORD with appropriate temperature rating used for ME EQUIPMENT having external metal parts with a temperature > 75 °C touchable by the cord in NORMAL USE :	See appended Table 8.10	N/A
8.11.3.3	NOMINAL cross-sectional area of conductors of POWER SUPPLY CORDS of ME EQUIPMENT is not less than in Table 17 (mm ² Cu)..... :	--	N/A
8.11.3.4	APPLIANCE COUPLERS complying with IEC 60320-1 are considered to comply with 8.11.3.5 and 8.11.3.6 :	See appended Table 8.10	N/A
8.11.3.5	Cord anchorage (for APPLIANCE COUPLERS not complying with IEC 60320-1)		N/A
	a) Conductors of POWER SUPPLY CORD provided with strain relieve and insulation protected from abrasion at point of entry to ME EQUIPMENT or a MAINS CONNECTOR by a cord anchorage	No power supply cord provided. EUT is intended for building-in.	N/A
	b) Cord anchorage of POWER SUPPLY CORD is made of and arranged as follows when a total insulation failure of POWER SUPPLY CORD caused conductive non-PROTECTIVELY EARTHED ACCESSIBLE PARTS to exceed limits of 8.4:	--	N/A
	– insulating material, or	--	N/A
	– metal, insulated from conductive ACCESSIBLE PARTS non-PROTECTIVELY EARTHED by a MEANS OF PROTECTION, or	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– metal provided with an insulating lining affixed to cord anchorage, except when it is a flexible bushing forming part of the cord guard in 8.11.3.6, and complying with the requirements for one MEANS OF PROTECTION	--	N/A
	c) Cord anchorage prevents cord from being clamped by a screw bearing directly on cord insulation	--	N/A
	d) Screws to be operated when replacing POWER SUPPLY CORD do not serve to secure any components other than parts of cord anchorage	--	N/A
	e) Conductors of POWER SUPPLY CORD arranged to prevent PROTECTIVE EARTH CONDUCTOR against strain as long as phase conductors are in contact with their terminals when cord anchorage fails	--	N/A
	f) Cord anchorage prevents POWER SUPPLY CORD from being pushed into ME EQUIPMENT or MAINS CONNECTOR	--	N/A
	Conductors of POWER SUPPLY CORD supplied by MANUFACTURER disconnected from terminals or from MAINS CONNECTOR and cord subjected 25 times to a pull applied with no jerks, each time for 1 s, on sheath of the value in Table 18:	See appended Table 8.11.3.5	N/A
	Cord subjected to a torque in Table 18 for 1 min immediately after pull tests	--	N/A
	Cord anchorage did not allow cord sheath to be longitudinally displaced by more than 2 mm or conductor ends to move over a distance of more than 1 mm from their connected position	--	N/A
	CREEPAGE and CLEARANCES not reduced below limits in 8.9	--	N/A
	It was not possible to push the cord into ME EQUIPMENT or MAINS CONNECTOR to an extent the cord or internal parts would be damaged	--	N/A
8.11.3.6	POWER SUPPLY CORDS other than for STATIONARY ME EQUIPMENT protected against excessive bending at inlet opening of equipment or of MAINS CONNECTOR by means of an insulating cord guard or by means of an appropriately shaped opening	No power supply cord provided. EUT is intended for building-in.	N/A
	Cord guard complied with test of IEC 60335-1:2001, Clause 25.14, or	--	N/A
	ME EQUIPMENT placed such that axis of cord guard projected at an angle of 45° with cord free from stress, and a mass equal 10 x D ² gram attached to the free end of cord (g).....:	See appended Table 8.11.3.6	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Cord guard of temperature-sensitive material tested at 23 °C ± 2 °C, and flat cords bent in the plane of least resistance	--	N/A
	Curvature of the cord radius, immediately after mass attached, was not less than 1.5 x D..... :	See appended Table 8.11.3.6	N/A
8.11.4	MAINS TERMINAL DEVICES		P
8.11.4.1	PERMANENTLY INSTALLED and ME EQUIPMENT with non-DETACHABLE POWER SUPPLY CORD replaceable by SERVICE PERSONNEL provided with MAINS TERMINAL DEVICES ensuring reliable connection	EUT is intended for building-in.	N/A
	Terminals alone are not used to keep conductors in position, except when barriers are provided such that CREEPAGE and CLEARANCES cannot be reduced below 8.9 if any conductor breaks away	Input connector used (for line and neutral). See enclosed pictures of the unit for details.	P
	Terminals of components other than terminal blocks complying with requirements of this Clause and marked according to 7.3.7 used as terminals intended for external conductors	--	N/A
	Screws and nuts clamping external conductors do not serve to secure any other component, except they also clamp internal conductors when unlikely to be displaced when fitting the supply conductors	--	N/A
8.11.4.2	Arrangement of MAINS TERMINAL DEVICES		P
	a) Terminals provided for connection of external cords or POWER SUPPLY CORDS together with PROTECTIVE EARTH TERMINAL grouped to provide convenient means of connection	Approved input connector provided. See enclosed pictures of the unit for details.	P
	b) PROTECTIVE EARTH CONDUCTOR connections complied with 8.6	Standard PE terminal provided.	P
	c) Marking of MAINS TERMINAL DEVICES complied with 7.3	--	N/A
	d) MAINS TERMINAL DEVICES not accessible without use of a TOOL	EUT is intended for building-in; therefore end product consideration.	N/A
	e) A MEANS OF PROTECTION are not short circuited when one end of a flexible conductor with NOMINAL cross-sectional area is stripped 8 mm and a single free wire is bent in each possible direction	--	N/A
8.11.4.3	Internal wiring not subjected to stress and CREEPAGE and CLEARANCES not reduced below 8.9 after fastening and loosening a conductor of largest cross-sectional area 10 times	Through the hole method in addition to soldering used for PE conductor. No other conductors within the equipment.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.11.4.4	Terminals with clamping means for a rewirable flexible cord did not require special preparation of conductors and conductors were not damaged and did not slip out when clamping means tightened as verified by test of 8.11.3.4	Approved input connector used for connection to the mains.	N/A
8.11.4.5	Adequate space provided inside ME EQUIPMENT designed for FIXED wiring or a re-wirable POWER SUPPLY CORD to allow for connection of conductors, and covers fitted without damage to conductors or their insulation	Approved input connector used for connection to the mains.	N/A
	Correct connection and positioning of conductors before ACCESS COVER was fitted verified by an installation test	--	N/A
8.11.5	Mains fuses and OVER-CURRENT RELEASES		P
	A fuse or OVER-CURRENT RELEASE provided in each supply lead for CLASS I and CLASS II ME EQUIPMENT with a functional earth connection per clause 8.6.9, and in at least one supply lead for other single-phase CLASS II ME EQUIPMENT.... :	See appended Table 8.10 and Appended RM Results Table 8.11.5 Two primary fuses provided (in both supply leads).	P
	– neutral conductor not fused for PERMANENTLY INSTALLED ME EQUIPMENT	Not permanently installed equipment.	N/A
	– fuses or OVER-CURRENT RELEASES omitted due to provision of two MEANS OF PROTECTION between all parts of opposite polarity within MAINS PART, and between all parts of MAINS PART and earth, and such provisions continued within all components	Input fuses provided.	N/A
	Effect of short-circuit fault conditions in other circuits taken into consideration before eliminating fuses or OVER-CURRENT RELEASES	--	N/A
	Protective devices have adequate breaking capacity to interrupt the maximum fault current including the available short-circuit	See appended Table 8.10	P
	A fuse or OVER-CURRENT RELEASE not provided in a PROTECTIVE EARTH CONDUCTOR	--	P
	Fuses complying with IEC 60127 have high breaking capacity (1 500 A) and prospective short-circuit current > 35 A or 10 times current rating of the fuse, whichever is greater	Input fuses operated during single fault testing without safety hazard.	P
	Justification for omission of fuses or OVER-CURRENT RELEASES is in RISK MANAGEMENT FILE	--	N/A
8.11.6	Internal wiring of the MAINS PART		P
	a) Cross-sectional area of internal wiring in a MAINS PART between MAINS TERMINAL DEVICE and protective devices is not less than minimum required for POWER SUPPLY CORD as in clause 8.11.3.3 (mm ² Cu)	No conductors provided.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	b) Cross-sectional area of other wiring in MAINS PART and sizes of tracks on printed wiring circuits sufficient to prevent fire in case of fault currents..... :	See appended Table 8.10 PCB tracks.	P
	When necessary, ME EQUIPMENT connected to a SUPPLY MAINS with max available short-circuit fault, and subsequent simulation of a fault in a single insulation in MAINS PART did not result in any of the HAZARDOUS SITUATIONS in 13.1.2	--	N/A

9	PROTECTION AGAINST MECHANICAL HAZARDS OF ME EQUIPMENT AND ME SYSTEMS		P
9.1	ME EQUIPMENT complies with Clause 4 for design and manufacture, and mechanical strength (15.3)	--	P
9.2	HAZARDS associated with moving parts		N/A
9.2.1	When ME EQUIPMENT with moving parts PROPERLY INSTALLED, used per ACCOMPANYING DOCUMENTS or under foreseeable misuse, RISKS associated with moving parts reduced to an acceptable level..... :	See Appended RM Results Table 9.2.1 No moving parts provided. External ventilation fan not part of the equipment. End product consideration.	N/A
	RISK from contact with moving parts reduced to an acceptable level using protective measures, (access, function, shape of parts, energy, speed of motion, and benefits to PATIENT considered)	--	N/A
	RESIDUAL RISK associated with moving parts considered acceptable when exposure was needed for ME EQUIPMENT to perform its function	--	N/A
	Warnings marked on ME EQUIPMENT or included in instructions for use when HAZARDS persisted after implementing all reasonable protective measures..... :	See provided Marking Labels	N/A
9.2.2	TRAPPING ZONE		N/A
9.2.2.1	ME EQUIPMENT with a TRAPPING ZONE complied with one or more of the following as feasible:	No trapping zones.	N/A
	– Gaps in Clause 9.2.2.2, or	--	N/A
	– Safe distances in Clause 9.2.2.3, or	--	N/A
	– GUARDS and protective measures in 9.2.2.4, or	--	N/A
	– Continuous activation in Clause 9.2.2.5	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Control of relevant motion complied with 9.2.2.6 when implementation of above protective measures were inconsistent with INTENDED USE of ME EQUIPMENT or ME SYSTEM	--	N/A
9.2.2.2	A TRAPPING ZONE considered not to present a MECHANICAL HAZARD when gaps of TRAPPING ZONE complied with dimensions per Table 20 . :	See appended Table 9.2.2.2	N/A
9.2.2.3	A TRAPPING ZONE considered not to present a MECHANICAL HAZARD when distances separating OPERATOR, PATIENT, and others from TRAPPING ZONES exceeded values in ISO 13852 :	See appended Table 9.2.2.2	N/A
	Distances measured from expected positions of OPERATOR, PATIENT, and others near EQUIPMENT in NORMAL USE or under foreseeable misuse	--	N/A
9.2.2.4	GUARDS and protective measures		N/A
9.2.2.4.1	A TRAPPING ZONE considered not to present a MECHANICAL HAZARD when GUARDS and protective measures were of robust construction, not easy to bypass or render non-operational, and did not introduce additional unacceptable RISK based on results of applicable tests in 15.3 for ENCLOSURES..... :	See Appended Table 15.3	N/A
9.2.2.4.2	FIXED GUARDS held in place by systems that cannot be dismantled without a TOOL	--	N/A
9.2.2.4.3	Movable GUARDS that can be opened without a TOOL remained attached when GUARD was open	See Appended RM Results Table 9.2.2.4.3	N/A
	– they are associated with an interlock preventing relevant moving parts from starting to move while TRAPPING ZONE is accessible, and stops movement when the GUARD is opened,	--	N/A
	– absence or failure of one of their components prevents starting, and stops moving parts	--	N/A
	Movable GUARDS complied with all applicable tests as confirmed by review of RISK MANAGEMENT FILE	--	N/A
9.2.2.4.4	Protective measures provided in control system prevented moving parts from starting to move while in reach of persons :	See Appended RM Results Table 9.2.2.4.4	N/A
	– protective measures prevented TRAPPING ZONE from reach, or, when it was reached, system movement stopped once ME EQUIPMENT started to move, and in the latter case, no HAZARD or damage resulted	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– when protective measure was in a SINGLE FAULT CONDITION, and an unacceptable RISK could arise, one or more emergency stopping device(s) provided	--	N/A
	RISK MANAGEMENT FILE reviewed and all conditions confirmed	--	N/A
9.2.2.5	Continuous activation		N/A
	TRAPPING ZONE not considered to present a MECHANICAL HAZARD where impractical to make TRAPPING ZONE inaccessible when:	--	N/A
	a) movement was in OPERATOR's field of view	--	N/A
	b) movement of ME EQUIPMENT or its parts was possible only by continuous activation of control by OPERATOR as long as OPERATOR response to deactivate device relied upon to prevent HARM	--	N/A
	Manually operated movements complied with this clause since mass and velocity allowed adequate control of positioning without causing an unacceptable RISK	--	N/A
	c) when in a SINGLE FAULT CONDITION of continuous activation system an unacceptable RISK could arise, one or more emergency stopping device(s) provided in ME EQUIPMENT ...:	See Appended RM Results Table 9.2.2.5 c)	N/A
9.2.2.6	Speed of movement(s) positioning parts of ME EQUIPMENT or PATIENT, when contact with ME EQUIPMENT could result in a HAZARDOUS SITUATION, limited to allow OPERATOR control of positioning without resulting in an unacceptable RISK:	See Appended RM Results Table 9.2.2.6	N/A
	Over travel (stopping distance) of such movement occurring after operation of a control to stop movement, did not result in an unacceptable RISK	--	N/A
9.2.3	Other HAZARDS associated with moving parts		N/A
9.2.3.1	Controls positioned, recessed, or protected by other means and could not be accidentally actuated to result in unacceptable RISK, except when ergonomic considerations for a PATIENT with special needs require otherwise	No moving parts. External ventilation fan not part of the equipment (used for 10 CFM air flow).	N/A
9.2.3.2	RISK due to over travel (past range limits) of ME EQUIPMENT parts reduced to an acceptable level, and stops or other means with mechanical strength to withstand intended loading in NORMAL USE and foreseeable misuse provided limiting measure in NORMAL and SINGLE FAULT CONDITION:	See appended Table 8.10 and Appended RM Results Table 9.2.3.2	N/A
9.2.4	Emergency stopping devices		N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Where necessary to have one or more emergency stopping device(s), emergency stopping device complied with all the following, except for actuating switch capable of interrupting all power	See Appended RM Results Table 9.2.4 No emergency stopping device provided.	N/A
	a) Emergency stopping device reduced RISK to an acceptable level	--	N/A
	b) Proximity and response of OPERATOR to actuate emergency stopping device could be relied upon to prevent HARM	--	N/A
	c) Emergency stopping device actuator was readily accessible to OPERATOR	--	N/A
	d) Emergency stopping device(s) are not part of normal operation of ME EQUIPMENT	--	N/A
	e) Emergency switching operation or stopping means neither introduced further HAZARD nor interfered with operation necessary to remove original HAZARD	--	N/A
	f) Emergency stopping device was able to break full load of relevant circuit, including possible stalled motor currents and the like	--	N/A
	g) Means for stopping of movements operate as a result of one single action	--	N/A
	h) Emergency stopping device provided with an actuator in red and easily distinguishable and identifiable from other controls	--	N/A
	i) An actuator interrupting/opening mechanical movements marked on or immediately adjacent to face of actuator with symbol 18 of Table D.1 (symbol IEC 60417-5638, DB:2002-10) or "STOP"	--	N/A
	j) Emergency stopping device, once actuated, maintained ME EQUIPMENT in disabled condition until a deliberate action, different from that used to actuate it, was performed	--	N/A
	k) Emergency stopping device is suitable for its application	--	N/A
9.2.5	Means provided to permit quick and safe release of PATIENT in event of breakdown of ME EQUIPMENT or failure of power supply, activation of a protective measure, or emergency stopping, and	See Appended RM Results Table 9.2.5	N/A
	– Uncontrolled or unintended movement of ME EQUIPMENT that could result in an unacceptable RISK prevented	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Situations where PATIENT is subjected to unacceptable RISKS due to proximity of moving parts, removal of normal exit routes, or other HAZARDS prevented	--	N/A
	– Measures provided to reduce RISK to an acceptable level when after removal of counterbalanced parts, other parts of ME EQUIPMENT can move in a hazardous way	--	N/A
9.3	Rough surfaces, sharp corners and edges of ME EQUIPMENT that could result in an unacceptable RISK avoided or covered	See Appended RM Results Table 9.3 No rough surfaces, no sharp corners and no sharp edges.	P
9.4	Instability HAZARDS		N/A
9.4.1	ME EQUIPMENT, other than FIXED and hand-held, for placement on a surface did not overbalance (tip over) or move unexpectedly, to the degree that it could present an unacceptable RISK to PATIENT, or OPERATOR as tested in 9.4.2 to 9.4.4	EUT is power supply unit intended for building-in.	N/A
9.4.2	Instability – overbalance		N/A
9.4.2.1	ME EQUIPMENT or its parts did not overbalance when prepared per ACCOMPANYING DOCUMENTS, or when not specified, as in 9.4.2.2, and placed on a 10° inclined plane from horizontal consisting of a hard and flat surface (e.g., concrete floor covered with 2 to 4 mm thick vinyl material)	See Appended Table 9.4.2.1	N/A
9.4.2.2	Instability excluding transport		N/A
	ME EQUIPMENT or its parts prepared based on a) to g), inclusive, did not overbalance when placed in different positions of NORMAL USE, except transport positions, on a 5° inclined plane from horizontal (hard and flat surface)	See Appended Table 9.4.2.2	N/A
	A warning provided, stating “Transport only under conditions described in instructions for use or marked on ME EQUIPMENT with an indication of RESIDUAL RISK if ME EQUIPMENT or its parts overbalances” when overbalance occurred during 10° inclined plane test	--	N/A
9.4.2.3	Instability from horizontal and vertical forces		N/A
	a) ME EQUIPMENT with a mass of 25 kg or more, other than FIXED ME EQUIPMENT for use on floor, did not overbalance due to pushing or resting	Mass of equipment less than 25 kg.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Surfaces of ME EQUIPMENT where a RISK of overbalancing exists from pushing, leaning, resting etc., permanently marked with a CLEARLY LEGIBLE warning of the RISK (e.g., safety sign 5 of Table D.2, safety sign ISO 7010-P017)	--	N/A
	ME EQUIPMENT did not overbalance when placed on a horizontal plane, and a force of 25% of its weight, but not more than 220 N, applied in different directions, except a direction with an upward component	--	N/A
	b) ME EQUIPMENT, other than FIXED ME EQUIPMENT, for use on the floor or on a table, did not overbalance due to sitting or stepping, except when a legible warning of this RISK provided on ME EQUIPMENT (e.g., safety signs 6 and 7 of Table D.2, safety signs ISO 7010-P018, or ISO 7010-P019 as appropriate)	--	N/A
	ME EQUIPMENT did not overbalance when placed on a horizontal plane, and a constant force of 800 N applied at the point of maximum moment to working surfaces, offering an foothold or sitting surface of a min 20 x 20 cm area, and at a height ≤ 1 m from the floor :	See Appended Table 9.4.2.3	N/A
9.4.2.4	Castors and wheels		N/A
9.4.2.4.1	Means used for transportation of MOBILE ME EQUIPMENT (e.g., castors or wheels) did not result in an unacceptable RISK when MOBILE ME EQUIPMENT moved or parked in NORMAL USE	--	N/A
9.4.2.4.2	Force required to move MOBILE ME EQUIPMENT along a hard and flat horizontal surface did not exceed 200 N applied at a height of 1 m above floor or highest point on ME EQUIPMENT when < 1 m high, except when instructions indicated more than one person needed (N) ... :	See Appended Table 9.4.2.4.2	N/A
9.4.2.4.3	MOBILE ME EQUIPMENT exceeding 45 kg configured with a SAFE WORKING LOAD, moved 10 times in forward direction over a solid vertical plane obstruction with wheels impacting the obstruction at a speed of 0.4 m/s \pm 0.1 m/s for manual or with max speed for motor driven MOBILE ME EQUIPMENT :	See Appended Table 9.4.2.4.3	N/A
	ME EQUIPMENT went up the obstruction without overbalancing or any other unacceptable RISK as determined by examination of RISK MANAGEMENT FILE, ME EQUIPMENT and its parts... :	See Appended RM Results Table 9.4.2.3	N/A
	There was no reduction of CREEPAGE and CLEARANCES below 8.9, no access to parts exceeding limits in 8.4, and no access to moving parts capable of causing HARM, and	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Assessment criteria in Clause 9 and 11.6 used	--	N/A
	– Dielectric strength test of 8.8.3 conducted to evaluate integrity of solid SUPPLEMENTARY or REINFORCED INSULATION	--	N/A
	– CREEPAGE DISTANCES and AIR CLEARANCES measured compared favourably with min distances in clause 8.9	--	N/A
	Small chips not adversely affecting protection against electric shock or moisture, disregarded	--	N/A
9.4.3	Instability from unwanted lateral movement (including sliding)		N/A
9.4.3.1	a) Brakes of power-driven MOBILE ME EQUIPMENT normally activated and could only be released by continuous actuation of a control	--	N/A
	b) MOBILE ME EQUIPMENT provided with locking means to prevent unwanted movements of ME EQUIPMENT or its parts in transport position	--	N/A
	c) No unacceptable RISK due to unwanted lateral movement resulted when MOBILE ME EQUIPMENT placed in its transport position or worst case NORMAL USE position with SAFE WORKING LOAD, and locking device activated, on a 10° inclined hard flat surface with castors in the worst-case position	--	N/A
	Following initial elastic movement, creepage, and pivoting of castors, no further movement of MOBILE ME EQUIPMENT > 50 mm (in relation to inclined plane) occurred (mm).....:	See Appended Table 9.4.3.1	N/A
	RISK due to any initial movement assessed taking into consideration NORMAL USE of ME EQUIPMENT	--	N/A
9.4.3.2	Instability excluding transport		N/A
	a) Further movement of ME EQUIPMENT (after initial elastic movement) was less than 50 mm when MOBILE ME EQUIPMENT with a SAFE WORKING LOAD positioned on a 5° inclined hard flat surface with wheel locked or braking system activated (mm).....:	See Appended Table 9.4.3.2	N/A
	RISK due to initial movements assessed taking into consideration NORMAL USE of ME EQUIPMENT	--	N/A
	b) TRANSPORTABLE or STATIONARY ME EQUIPMENT for use on the floor and with a SAFE WORKING LOAD prepared as in 9.4.2.2 and placed on a horizontal plane with locking device activated and castors, when supplied, in their worst – case position	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Further movement of ME EQUIPMENT (after initial elastic movement), was no more than 50 mm when a force of 25 % of weight of unit, but less than 220 N, applied in different directions, except a direction with an upwards component, at highest point of ME EQUIPMENT but ≤ 1.5 m from floor.....:	See Appended Table 9.4.3.2	N/A
	RISK due to initial movements assessed taking into consideration NORMAL USE of ME EQUIPMENT	--	N/A
9.4.4	Grips and other handling devices		N/A
	a) ME EQUIPMENT other than PORTABLE EQUIPMENT or its part with a mass of over 20 kg requiring lifting in NORMAL USE or transport provided with suitable handling means, or ACCOMPANYING DOCUMENTS specify safe lifting method, except when handling is obvious and causing HAZARDS	--	N/A
	Handles, when supplied, suitably placed to enable ME EQUIPMENT or its part to be carried by two or more persons and by examination of EQUIPMENT, its part, or ACCOMPANYING DOCUMENTS	--	N/A
	b) PORTABLE ME EQUIPMENT with a mass > 20 kg provided with one or more carrying-handles suitably placed to enable carrying by two or more persons as confirmed by actual carrying	--	N/A
	c) Carrying handles and grips and their means of attachment withstood loading test.....:	See Appended Table 9.4.4	N/A
9.5	Expelled parts HAZARD		N/A
9.5.1	Suitability of means of protecting against unacceptable RISK of expelled parts determined by assessment and examination of RISK MANAGEMENT FILE..... :	See Appended RM Results Table 9.5.1 No expelled parts can occur.	N/A
9.5.2	Cathode ray tube(s) complied with IEC 60065:2001, Clause 18, or IEC 61965..... :	See appended Table 8.10	N/A
9.6	Acoustic energy (including infra- and ultrasound) and vibration		N/A
9.6.1	Human exposure to acoustic energy and vibration from ME EQUIPMENT doesn't result in unacceptable RISK as confirmed in RISK MANAGEMENT FILE including audibility of auditory alarm signals, PATIENT sensitivity, and tests of 9.6.2 and 9.6.3 :	See Appended RM Results Table 9.6.1 EUT not produces acoustic energy or vibration.	N/A
9.6.2	Acoustic energy		N/A
9.6.2.1	PATIENT, OPERATOR, and other persons are not exposed to acoustic energy from ME EQUIPMENT in NORMAL USE, except for auditory alarm signals	EUT not produces acoustic energy.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– 80 dBA for a cumulative exposure of 24 h over a 24 h period (dBA).....:	--	—
	- 83 dBA (when halving the cumulative exposure time) (dBA).....:	--	—
	– 140 dB un-weighted sound pressure level for impulsive or impact acoustic energy (dB).....:	--	—
9.6.2.2	RISK MANAGEMENT FILE examined for RISKS associated with infrasound or ultrasound, when present, addressed in RISK MANAGEMENT PROCESS	See Appended RM Results Table 9.6.2.2	N/A
9.6.3	Hand-transmitted vibration		N/A
	Means provided, except for INTENDED USE vibrations, to protect PATIENT and OPERATOR when hand-transmitted frequency-weighted r.m.s. acceleration generated in NORMAL USE exceeds specified values measured at points of hand contact with PATIENT or OPERATOR	EUT not hand-held equipment.	N/A
	– 2.5 m/s ² for a cumulative time of 8 h during a 24 h period (m/s ²)	--	N/A
	– Accelerations for different times, inversely proportional to square root of time (m/s ²)	--	N/A
9.7	Pressure vessels and parts subject to pneumatic and hydraulic pressure		N/A
9.7.1	Requirements of this clause applied to vessels and parts of ME EQUIPMENT subject to pressure resulting in rupture and unacceptable RISK	No pressure vessels or parts subject to pressure provided.	N/A
	Parts of a pneumatic or hydraulic system used as a support system, comply with 9.8	--	N/A
9.7.2	Pneumatic and hydraulic parts of ME EQUIPMENT or ACCESSORIES met following requirements based on examination of RISK MANAGEMENT FILE	See Appended RM Results Table 9.7.2 No pneumatic and hydraulic parts within the equipment.	N/A
	– No unacceptable RISK resulted from loss of pressure or loss of vacuum	--	N/A
	– No unacceptable RISK resulted from a fluid jet caused by leakage or a component failure	--	N/A
	– Elements of ME EQUIPMENT or an ACCESSORY, especially pipes and hoses leading to an unacceptable RISK protected against harmful external effects	--	N/A
	– Reservoirs and similar vessels leading to an unacceptable RISK are automatically depressurized when ME EQUIPMENT is isolated from its power supply	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Means provided for isolation, or local depressurizing reservoirs and similar vessels, and pressure indication when above not possible	--	N/A
	– All elements remaining under pressure after isolation of ME EQUIPMENT or an ACCESSORY from its power supply resulting in an unacceptable RISK provided with clearly identified exhaust devices, and a warning to depressurize these elements before setting or maintenance activity	--	N/A
9.7.3	Maximum pressure a part of ME EQUIPMENT can be subjected to in NORMAL and SINGLE FAULT CONDITIONS considered to be highest of following:	--	N/A
	a) RATED maximum supply pressure from an external source	--	N/A
	b) Pressure setting of a pressure-relief device provided as part of assembly	--	N/A
	c) Max pressure that can develop by a source of pressure that is part of assembly, unless pressure limited by a pressure-relief device	--	N/A
9.7.4	Max pressure in NORMAL and SINGLE FAULT CONDITIONS did not exceed MAXIMUM PERMISSIBLE WORKING PRESSURE for EQUIPMENT part, except as allowed in 9.7.7, confirmed by examination of ME EQUIPMENT and RISK MANAGEMENT FILE, and by functional tests..... :	See Appended RM Results Table 9.7.4	N/A
9.7.5	A pressure vessel withstood a HYDRAULIC TEST PRESSURE when pressure was > 50 kPa, and product of pressure and volume was more than 200 kPa..... :	See Appended Table 9.7.5	N/A
9.7.6	Pressure-control device regulating pressure in ME EQUIPMENT with pressure-relief device completed 100,000 cycles of operation under RATED load and prevented pressure from exceeding 90 % of setting of pressure-relief device in different conditions of NORMAL USE . :	See Appended RM Results Table 9.7.6 No such devices incorporated.	N/A
9.7.7	Pressure-relief device(s) used where MAXIMUM PERMISSIBLE WORKING PRESSURE could otherwise be exceeded met the following, as confirmed by MANUFACTURER'S data, ME EQUIPMENT, RISK MANAGEMENT FILE, and functional tests :	See Appended RM Results Table 9.7.7 No pressure-relief devices provided.	N/A
	a) Connected as close as possible to pressure vessel or parts of system it is to protect	--	N/A
	b) Installed to be readily accessible for inspection, maintenance, and repair	--	N/A
	c) Could be adjusted or rendered inoperative without a TOOL	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	d) With discharge opening located and directed as to not to release material towards any person	--	N/A
	e) With discharge opening located and directed as to not to deposit material on parts that could result in an unacceptable RISK	--	N/A
	f) Adequate discharge capacity provided to ensure that pressure will not exceed MAXIMUM PERMISSIBLE WORKING PRESSURE of system it is connected to by more than 10 % when failure occurs in control of supply pressure	--	N/A
	g) No shut-off valve provided between a pressure-relief device and parts it is to protect	--	N/A
	h) Min number of cycles of operation 100 000, except for one-time use devices (bursting disks)	--	N/A
9.8	HAZARDS associated with support systems		N/A
9.8.1	ME EQUIPMENT parts designed to support loads or provide actuating forces when a mechanical fault could constitute an unacceptable RISK	See appended Table 8.10 and Appended RM Results Table 9.8.1 EUT is not intended to support loads.	N/A
	– Construction of support, suspension, or actuation system complied with Table 21 and TOTAL LOAD	--	N/A
	– Means of attachment of ACCESSORIES prevent possibility of incorrect attachment that could result in an unacceptable RISK	--	N/A
	– RISK ANALYSIS of support systems included HAZARDS from static, dynamic, vibration, impact and pressure loading, foundation and other movements, temperature, environmental, manufacture and service conditions	--	N/A
	– RISK ANALYSIS included effects of failures such as excessive deflection, plastic deformation, ductile/brittle fracture, fatigue fracture, instability (buckling), stress-assisted corrosion cracking, wear, material creep and deterioration, and residual stresses from manufacturing PROCESSES	--	N/A
	– Instructions on attachment of structures to a floor, wall, ceiling, included in ACCOMPANYING DOCUMENTS making adequate allowances for quality of materials used to make the connection and list the required materials	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Additional instructions provided on checking adequacy of surface of structure parts will be attached to	--	N/A
9.8.2	Support systems maintain structural integrity during EXPECTED SERVICE LIFE, and TENSILE SAFETY FACTORS are not less than in Table 21, except when an alternative method used to demonstrate structural integrity throughout EXPECTED SERVICE LIFE, or for a foot rest	--	N/A
	Compliance with 9.8.1 and 9.8.2 confirmed by examination of ME EQUIPMENT, RISK MANAGEMENT FILE, specifications and material processing.. :	See Appended RM Results Table 9.8.2	N/A
	When test results were part of information, testing consisted of application of a test load to support assembly equal to TOTAL LOAD times required TENSILE SAFETY FACTOR while support assembly under test was in equilibrium after 1 min, or not resulted in an unacceptable RISK . :	See appended Table 8.10	N/A
9.8.3	Strength of PATIENT or OPERATOR support or suspension systems		N/A
9.8.3.1	ME EQUIPMENT parts supporting or immobilizing PATIENTS minimize RISK of physical injuries and accidental loosening of secured joints	See Appended RM Results Table 9.8.3.1	N/A
	SAFE WORKING LOAD of ME EQUIPMENT or its parts supporting or suspending PATIENTS or OPERATORS is sum of mass of PATIENTS or mass of OPERATORS plus mass of ACCESSORIES supported by ME EQUIPMENT or its parts	--	N/A
	Supporting and suspending parts for adult human PATIENTS or OPERATORS designed for a PATIENT or OPERATOR with a min mass of 135 kg and ACCESSORIES with a min mass of 15 kg, unless stated by MANUFACTURER	--	N/A
	Maximum mass of PATIENT included in SAFE WORKING LOAD of ME EQUIPMENT or its parts supporting or suspending PATIENTS adapted when MANUFACTURER specified applications	--	N/A
	Max allowable PATIENT mass < 135 kg marked on ME EQUIPMENT and stated in ACCOMPANYING DOCUMENTS	--	N/A
	Max allowable PATIENT mass > 135 kg stated in ACCOMPANYING DOCUMENTS	--	N/A
	Examination of markings, ACCOMPANYING DOCUMENTS, and RISK MANAGEMENT FILE confirmed compliance :	See copy of Marking Label	N/A
9.8.3.2	Part of SAFE WORKING LOAD representing mass of PATIENTS or OPERATORS is distributed on support/suspension surface representing human body as in Fig A.19	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Part of SAFE WORKING LOAD representing mass of ACCESSORIES deployed as in NORMAL USE and, when not defined, at worst case position permitted by configuration or ACCESSORIES attachment on support/suspension parts	--	N/A
	a) Entire mass of PATIENT or OPERATOR distributed over an area of 0.1 m ² on a foot rest temporarily supporting a standing PATIENT or OPERATOR	See Appended RM Results Table 9.8.3.2 a)	N/A
	Compliance confirmed by examination of ME EQUIPMENT, RISK MANAGEMENT FILE, specifications of materials and their processing, and tests	See appended Table 8.10	N/A
	PATIENT support/suspension system positioned horizontally in most disadvantageous position in NORMAL USE, and a mass 2 x 135 kg or twice intended person's load (the greater used), applied to foot rest over an area of 0.1 m ² for 1 min (Kg).....	See appended Table 9.8.3.2	N/A
	Damage or deflection resulting in an unacceptable RISK did not occur on foot rest and its secured joints	--	N/A
	b) Deflection of a support surface from PATIENT or OPERATOR loading on an area of support/ suspension where a PATIENT or OPERATOR can sit did not result in an unacceptable RISK.....	See Appended RM Results Table 9.8.3.2 b)	N/A
	Compliance confirmed by examination of ME EQUIPMENT, RISK MANAGEMENT FILE, specifications of materials and their processing, and by a test	See appended Table 8.10	N/A
	PATIENT support/suspension system set in most unfavourable NORMAL USE position, and a mass of 60 % of part of SAFE WORKING LOAD simulating PATIENT or OPERATOR, or a min 80 kg, placed on support or suspension system with centre of load 60 mm from outer edge of support or suspension system for at least one minute (Kg)	See appended Table 9.8.3.2	N/A
	Deflection of support/suspension system resulting in an unacceptable RISK not occur	--	N/A
9.8.3.3	Dynamic forces that can be exerted on equipment parts supporting or suspending a PATIENT or OPERATOR in NORMAL USE did not result in an unacceptable RISK as confirmed by following test:	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	PATIENT support/suspension system set in most unfavourable NORMAL USE position, and a mass equal to SAFE WORKING LOAD simulating PATIENT or OPERATOR dropped from 150 mm above seat area on an area of support/suspension a PATIENT or OPERATOR can sit.....:	See appended Table 9.8.3.3	N/A
9.8.4	Systems with MECHANICAL PROTECTIVE DEVICES		N/A
9.8.4.1	a) A MECHANICAL PROTECTIVE DEVICE provided when a support system or its parts impaired by wear have a TENSILE SAFETY FACTOR \geq to values in Table 21, rows 5 and 6, but less than 3 and 4	See Appended RM Results Table 9.8.4.1 EUT is medical direct plug-in power supply unit.	N/A
	b) MECHANICAL PROTECTIVE complies with the requirements as follows:	--	N/A
	– Designed based on TOTAL LOAD, and includes effects of SAFE WORKING LOAD when applicable	--	N/A
	– Has TENSILE SAFETY FACTORS for all parts not less than Table 21, row 7	--	N/A
	– Activated before travel (movement) produced an unacceptable RISK	--	N/A
	– Takes into account Clauses 9.2.5 and 9.8.4.3	--	N/A
	Compliance confirmed by examination of ME EQUIPMENT, RISK MANAGEMENT FILE, specifications of materials and their processing	See appended Table 8.10	N/A
9.8.4.2	Activation of MECHANICAL PROTECTIVE DEVICE is made obvious to OPERATOR when ME EQUIPMENT can still be used after failure of suspension or actuation means and activation of a MECHANICAL PROTECTIVE DEVICE (e.g., a secondary cable)	--	N/A
	MECHANICAL PROTECTIVE DEVICE requires use of a TOOL to be reset or replaced	--	N/A
9.8.4.3	MECHANICAL PROTECTIVE DEVICE intended to function once		N/A
	– Further use of ME EQUIPMENT not possible until replacement of MECHANICAL PROTECTIVE DEVICE	See Appended RM Results Table 9.8.4.3	N/A
	– ACCOMPANYING DOCUMENTS instruct once MECHANICAL PROTECTIVE DEVICE is activated, SERVICE PERSONNEL shall be called, and MECHANICAL PROTECTIVE DEVICE must be replaced before ME EQUIPMENT can be used	--	N/A
	– ME EQUIPMENT permanently marked with safety sign 2 of Table D.2 (i.e., safety sign 7010-W001)	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Marking is adjacent to MECHANICAL PROTECTIVE DEVICE or its location relative to MECHANICAL PROTECTIVE DEVICE is obvious to service personnel	--	N/A
	– Compliance confirmed by examination of ME EQUIPMENT, ACCOMPANYING DOCUMENTS, RISK MANAGEMENT FILE, specifications and processing of materials, and following test.....:	See appended Table 8.10	N/A
	A chain, cable, band, spring, belt, jack screw nut, pneumatic or hydraulic hose, structural part or the like, employed to support a load, defeated by a convenient means causing maximum normal load to fall from most adverse position permitted by construction of ME EQUIPMENT	--	N/A
	Load included SAFE WORKING LOAD in 9.8.3.1 when system was capable of supporting a PATIENT or OPERATOR	--	N/A
	No evidence of damage to MECHANICAL PROTECTIVE DEVICE affecting its ability to perform its intended function	--	N/A
9.8.5	Systems without MECHANICAL PROTECTIVE DEVICES		N/A
	Support system parts have TENSILE SAFETY FACTORS \geq to values in Table 21, rows 1 and 2, and are not impaired by wear	See Appended RM Results Table 9.8.5	N/A
	Support system parts impaired by wear, however, they have TENSILE SAFETY FACTORS \geq to values in Table 21, rows 3 and 4	--	N/A
	Examination of ME EQUIPMENT and RISK MANAGEMENT FILE confirmed compliance	--	N/A

10	PROTECTION AGAINST UNWANTED AND EXCESSIVE RADIATION HAZARDS		N/A
10.1	X-Radiation		N/A
10.1.1	X-radiation dose-rate was $\leq 36 \mu\text{A/kg}$ ($5 \mu\text{Sv/h}$) (0.5 mR/h) 5 cm from surface of ME EQUIPMENT including background radiation for ME EQUIPMENT not producing therapeutic/diagnostic X-radiation but producing ionizing radiation .:	See Table 10.1.1 EUT not produces X-radiation.	N/A
	Amount of radiation measured by means of an ionizing chamber radiation monitor with an effective area of 10 cm^2 or by other instruments producing equal results	--	N/A
	ME EQUIPMENT operated as in NORMAL USE at most unfavourable RATED MAINS VOLTAGE and controls adjusted to emit maximum radiation	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Internal pre-set controls not intended for adjustment during EXPECTED SERVICE LIFE of ME EQUIPMENT not taken into consideration	--	N/A
10.1.2	RISK from unintended X-radiation from ME EQUIPMENT producing X-radiation for diagnostic and therapeutic purposes addressed in RISK MANAGEMENT PROCESS as indicated in RISK MANAGEMENT FILE (see IEC 60601-1-3 & 1.3)	See Appended RM Results Table 10.1.2	N/A
10.2	RISK associated with alpha, beta, gamma, neutron, and other particle radiation, when applicable, addressed in RISK MANAGEMENT PROCESS as shown in RISK MANAGEMENT FILE	See Appended RM Results Table 10.2 EUT not produces alpha, beta, gamma, neutron and other radiation.	N/A
10.3	RISK associated with microwave radiation, when applicable, addressed in RISK MANAGEMENT PROCESS as indicated in RISK MANAGEMENT FILE	See Appended RM Results Table 10.3 EUT not produces microwave radiation.	N/A
10.4	Relevant requirements of IEC 60825-1:1993 applied to lasers, light emitting diodes (LEDs), and laser light barriers or similar products	No such components incorporated within the equipment.	N/A
10.5	RISK associated with visible electromagnetic radiation other than emitted by lasers and LEDs, when applicable, addressed in RISK MANAGEMENT PROCESS as indicated in RISK MANAGEMENT FILE	See Appended RM Results Table 10.5 EUT not produces electromagnetic radiation.	N/A
10.6	RISK associated with infrared radiation other than emitted by lasers and LEDs, as applicable, addressed in RISK MANAGEMENT PROCESS as indicated in RISK MANAGEMENT FILE	See Appended RM Results Table 10.6 EUT not produces infrared radiation.	N/A
10.7	RISK associated with ultraviolet radiation other than emitted by lasers and LEDs, as applicable, addressed in RISK MANAGEMENT PROCESS as indicated in RISK MANAGEMENT FILE	See Appended RM Results Table 10.7 EUT not produces ultraviolet radiation.	N/A
11	PROTECTION AGAINST EXCESSIVE TEMPERATURES AND OTHER HAZARDS		P
11.1	Excessive temperatures in ME EQUIPMENT		P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
11.1.1	Temperatures on ME EQUIPMENT parts did not exceed values in Tables 22 and 23 operating in worst-case NORMAL USE at maximum rated ambient operating temperature T :	See appended Table 11.1.1 and appended RM Results Table 11.1.1 Temperature tests performed in horizontal position without air flow (max. 65 W) and with 10 CFM air flow (max. 80 W). The risk management requirements of the standard were not addressed.	P
	Surfaces of test corner did not exceed 90 °C	Temperature of test corner not exceeds 90°C in normal conditions.	P
	THERMAL CUT-OUTS did not operate in NORMAL CONDITION	No thermal cut-outs incorporated.	N/A
11.1.2	Temperature of APPLIED PARTS		N/A
11.1.2.1	Temperatures, hot or cold surfaces, and when appropriate, clinical effects of APPLIED PARTS supplying heat to a PATIENT determined and documented in RISK MANAGEMENT FILE and instructions for use :	See appended Table 11.1.2.1 and appended RM Results Table 11.1.2.1 No applied parts.	N/A
11.1.2.2	APPLIED PARTS not supplying heat to a PATIENT met Table 24 with max surface temperatures > 41 °C disclosed in instructions for use, and clinical effects regarding maturity of PATIENTS, body surface, surface pressure, medications taken, as shown in RISK MANAGEMENT FILE :	See appended Table 11.1.2.2 and appended RM Results Table 11.1.2.2	N/A
	Surfaces of APPLIED PARTS cooled below ambient temperatures that can also result in HAZARD evaluated as part of RISK MANAGEMENT PROCESS	--	N/A
11.1.3	Measurements not made when engineering judgment and rationale by MANUFACTURER indicated temperature limits could not exceed, as documented in RISK MANAGEMENT FILE :	See appended Table 11.1.3 and RM Results Table 11.1.3 Temperature measurements performed.	N/A
	Test corner not used where engineering judgment and rationale by MANUFACTURER indicated test corner will not impact measurements, as documented in RISK MANAGEMENT FILE	Test corner used.	N/A
	Probability of occurrence and duration of contact for parts likely to be touched and for APPLIED PARTS documented in RISK MANAGEMENT FILE	The risk management requirements of the standard were not addressed.	N/A
11.1.4	GUARDS preventing contact with hot or cold accessible surfaces removable only with a TOOL	--	N/A
11.2	Fire prevention		P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
11.2.1	ENCLOSURE has strength and rigidity necessary to prevent a fire caused by reasonably foreseeable misuse and met mechanical strength tests for ENCLOSURES in 15.3	See clause 15.3.	P
11.2.2	Me equipment and me systems used in conjunction with OXYGEN RICH ENVIRONMENTS		N/A
11.2.2.1	RISK of fire in an OXYGEN RICH ENVIRONMENT reduced by means limiting spread of fire under NORMAL OR SINGLE FAULT CONDITIONS when source of ignition in contact with ignitable material ...:	See appended Table 8.10 EUT is not intended for use in conjunction with oxygen rich environment.	N/A
	Requirements of 13.1.1 applied to oxygen concentrations up to 25 % at one atmosphere or partial pressures up to 27.5 kPa for higher atmospheric pressures	--	N/A
	a) No sources of ignition discovered in an OXYGEN RICH ENVIRONMENT in NORMAL and SINGLE FAULT CONDITIONS under any of the following conditions	--	N/A
	1) when temperature of material raised to its ignition temperature	--	N/A
	2) when temperatures affected solder or solder joints causing loosening, short circuiting, or other failures causing sparking or increasing material temperature to its ignition temperature	--	N/A
	3) when parts affecting safety cracked or changed outer shape exposing temperatures higher than 300°C or sparks due to overheating	--	N/A
	4) when temperatures of parts or components exceeded 300°C, atmosphere was 100 % oxygen, contact material solder, and fuel cotton	--	N/A
	5) when sparks provided adequate energy for ignition by exceeding limits of Figs 35 to 37 (inclusive), atmosphere was 100 % oxygen, contact material solder, and fuel cotton	--	N/A
	Deviations from worst case limits in 4) and 5) above based on lower oxygen concentrations or less flammable fuels justified and documented in RISK MANAGEMENT FILE	See Appended RM Results Table 11.2.2.1	N/A
	Alternative test in this clause did not identify existence of ignition sources at highest voltage or current, respectively.....:	See appended Table 11.2.2.1	N/A
	A safe upper limit determined by dividing upper limit of voltage or current, respectively, with safety margin factor of three	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	b) RESIDUAL RISK of fire in an OXYGEN RICH ENVIRONMENT as determined by application of RISK MANAGEMENT PROCESS is based on following configurations, or in combination :	See Appended RM Results Table 11.2.2.1	N/A
	1) Electrical components in an OXYGEN RICH ENVIRONMENT provided with power supplies having limited energy levels lower than those considered sufficient for ignition in 11.2.2.1 a) as determined by examination, measurement or calculation of power, energy, and temperatures in NORMAL and SINGLE FAULT CONDITIONS identified in 11.2.3..... :	See appended Tables 4.11, 11.1.1 to 11.1.2.2, inclusive; and Table 13.2	N/A
	2) Max oxygen concentration measured until it did not exceed 25 % in ventilated compartments with parts that can be a source of ignition only in SINGLE FAULT CONDITION and can be penetrated by oxygen due to an undetected leak (%) :	--	N/A
	3) A compartment with parts or components that can be a source of ignition only under SINGLE FAULT CONDITION separated from another compartment containing an OXYGEN RICH ENVIRONMENT by sealing all joints and holes for cables, shafts, or other purposes	--	N/A
	Effect of possible leaks and failures under SINGLE FAULT CONDITION that could cause ignition evaluated using a RISK ASSESSMENT to determine maintenance intervals by examination of documentation and RISK MANAGEMENT FILE..... :	See Attachment #	N/A
	4) Fire initiated in ENCLOSURE of electrical components in a compartment with OXYGEN RICH ENVIRONMENT that can become a source of ignition only under SINGLE FAULT CONDITIONS self-extinguished rapidly and no hazardous amount of toxic gases reached PATIENT as determined by analysis of gases :	See Attachment #	N/A
11.2.2.2	RISK of ignition under least favourable conditions did not occur and oxygen concentration did not exceed 25% in immediate surroundings due to location of external exhaust outlets of an OXYGEN RICH ENVIRONMENT when electrical components mounted outside of ME EQUIPMENT or ME SYSTEM	--	N/A
11.2.2.3	Electrical connections within a compartment containing an OXYGEN RICH ENVIRONMENT under NORMAL USE did not produce sparks due to loosening or breaking, except when limited in power and energy to values in 11.2.2.1 a) 5)	--	N/A
	– Screw-attachments protected against loosening during use by varnishing, use of spring washers, or adequate torques	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Soldered, crimped, and pin-and-socket connections of cables exiting ENCLOSURE include additional mechanical securing means	--	N/A
11.2.3	SINGLE FAULT CONDITIONS related to OXYGEN RICH ENVIRONMENTS ME EQUIPMENT and ME SYSTEMS considered		N/A
	– Failure of a ventilation system constructed in accordance with 11.2.2.1 b) 2)	--	N/A
	– Failure of a barrier constructed in accordance with 11.2.2.1 b) 3)	--	N/A
	– Failure of a component creating a source of ignition (as defined in 11.2.2.1 a)	--	N/A
	– Failure of solid insulation or creepage and clearances providing equivalent of at least one MEANS OF PATIENT PROTECTION but less than two MEANS OF PATIENT PROTECTION that could create a source of ignition defined in 11.2.2.1 a)	--	N/A
	– Failure of a pneumatic component resulting in leakage of oxygen-enriched gas	--	N/A
11.3	Constructional requirements for fire ENCLOSURES of ME EQUIPMENT		N/A
	ME EQUIPMENT met this clause for alternate means of compliance with selected HAZARDOUS SITUATIONS and fault conditions in 13.1.2	See Appended RM Results Table 11.3 Power supply unit is intended for building-in. No external enclosure provided. See enclosed pictures of the unit for details.	N/A
	Constructional requirements were met, or	--	N/A
	- constructional requirements specifically analysed in RISK MANAGEMENT FILE	See Appended RM Results Table 11.3	N/A
	Justification, when requirement not met.....	--	N/A
	a) Flammability classification of insulated wire within fire ENCLOSURE is FV-1, or better, based on IEC 60695 series as determined by examination of data on materials	See appended Table 8.10	N/A
	Flammability classification of connectors, printed circuit boards, and insulating material on which components are mounted is FV-2, or better, based on IEC 60695-11-10 as decided by examination of materials data	See appended Table 8.10 PCB is rated UL94-V0.	N/A
	If no FV Certification, FV tests based on IEC 60695-11-10 conducted on 3 samples of complete parts (or sections of it), including area with min. thickness, ventilation openings	--	N/A
	b) Fire ENCLOSURE met following:	No external enclosure provided.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	1) No openings at bottom or, as specified in Fig 39, constructed with baffles as in Fig 38, or made of perforated metal as in Table 25, or a metal screen with a mesh $\leq 2 \times 2$ mm centre to centre and wire diameter of at least 0.45 mm	--	N/A
	2) No openings on the sides within the area included within the inclined line C in Fig 39	--	N/A
	3) ENCLOSURE, baffles, and flame barriers have adequate rigidity and made of appropriate metal or of non-metallic materials, except constructions based on Table 25 and a mesh; FV-2 or better for TRANSPORTABLE ME EQUIPMENT, FV-1 or better for fixed EQUIPMENT, or STATIONARY EQUIPMENT per IEC 60695-11-10, determined by ENCLOSURE examination or flammability classification based on 11.3a)..... :	See appended Table 8.10	N/A
11.4	ME EQUIPMENT and ME SYSTEMS intended for use with flammable anaesthetics		N/A
	ME EQUIPMENT, ME SYSTEMS and parts described in ACCOMPANYING DOCUMENTS for use with flammable anaesthetics (CATEGORY AP) or anaesthetics with oxidants (CATEGORY APG) comply with Annex G	EUT is not intended for use with flammable anaesthetics.	N/A
11.5	ME EQUIPMENT and ME SYSTEMS intended for use in conjunction with flammable agents		N/A
	MANUFACTURER'S RISK MANAGEMENT PROCESS addresses possibility of fire and associated mitigations as confirmed by examination of RISK MANAGEMENT FILE :	See Appended RM Results Table 11.5 EUT is not intended for use in conjunction with flammable agents.	N/A
11.6	Overflow, spillage, leakage, ingress of water or particulate matter, cleaning, disinfection, sterilization and compatibility with substances used with the ME EQUIPMENT		N/A
11.6.1	Sufficient degree of protection provided against overflow, spillage, leakage, ingress of water or particulate matter, cleaning, disinfection and sterilization, and compatibility with substances used with ME EQUIPMENT..... :	See Appended Table 11.6.1	N/A
11.6.2	Overflow in ME EQUIPMENT	No liquid reservoir provided.	N/A
	Liquid reservoir liable to overflow in NORMAL USE completely filled and 15 % of its capacity poured in for over 1 min, and except when restricted, TRANSPORTABLE ME EQUIPMENT tilted through an angle of 15° in least favourable direction(s), and when necessary refilled starting from position of NORMAL USE..... :	See Appended RM Results Table 11.6.2 and Table 11.6	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	ME EQUIPMENT met dielectric strength and LEAKAGE CURRENT tests and uninsulated electrical parts or electrical insulation of parts that could result in a HAZARDOUS SITUATION were not wet..... :	See appended Table 8.7 and 8.8.3	N/A
11.6. 3	Spillage on ME EQUIPMENT and ME SYSTEM	No liquid use.	N/A
	ME EQUIPMENT and ME SYSTEMS handling liquids in NORMAL USE positioned as in 5.4 a) and liquid with composition, volume, duration of spill, point of contact, and test conditions based on RISK MANAGEMENT PROCESS poured steadily on a point on top of ME EQUIPMENT..... :	See Appended RM Results Table 11.6.3 and Table 11.6	N/A
	ME EQUIPMENT met dielectric strength and LEAKAGE CURRENT tests and uninsulated electrical parts or electrical insulation of parts that could result in a HAZARDOUS SITUATION were not wet	See appended Tables 8.7 8.8.3	N/A
11.6.4	Leakage	See 13.2.6 No liquids used during normal use of the equipment.	N/A
11.6.5	Ingress of water or particulate matter into ME EQUIPMENT and ME SYSTEMS		N/A
	ME EQUIPMENT with IP Code placed in least favourable position of NORMAL USE and subjected to tests of IEC 60529 (IP Code)	See Appended RM Results Table 11.6.5 and Table 11.6 No protection against ingress of water provided. No external enclosure provided.	N/A
	ME EQUIPMENT met dielectric strength and LEAKAGE CURRENT tests and there were no bridging of insulation or electrical components that could result in a HAZARDOUS SITUATION in NORMAL CONDITION or in a SINGLE FAULT CONDITION	See appended Tables 8.7 8.8.3	N/A
11.6.6	Cleaning and disinfection of ME EQUIPMENT and ME SYSTEMS		N/A
	ME EQUIPMENT/ME SYSTEM and their parts and ACCESSORIES cleaned or disinfected once using methods specified in instructions for use including any cooling or drying period	See Appended RM Results Table 11.6.6 and Table 11.6 EUT is intended for building-in. End product consideration.	N/A
	ME EQUIPMENT met dielectric strength and LEAKAGE CURRENT tests, with no deterioration resulting in an unacceptable RISK present..... :	See appended Tables 8.7 8.8.3	N/A
	Effects of multiple cleanings/disinfections during EXPECTED SERVICE LIFE of EQUIPMENT evaluated by MANUFACTURER and assurance that no unacceptable RISK will occur verified by RISK MANAGEMENT FILE review	See RM Results Table 11.6.6	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
11.6.7	Sterilization of ME EQUIPMENT and ME SYSTEMS		N/A
	ME EQUIPMENT, ME SYSTEMS and their parts or ACCESSORIES intended to be sterilized assessed and documented according to ISO 11134, ISO 11135, or ISO 11137 as appropriate	See Appended RM Results Table 11.6.7	N/A
	After the test, ME EQUIPMENT complied with the appropriate dielectric strength and LEAKAGE CURRENT tests and there was no deterioration resulting in an unacceptable RISK	See appended Tables 8.7 8.8.3, and 11.6	N/A
11.6.8	RISKS associated with compatibility of substances used with ME EQUIPMENT addressed in RISK MANAGEMENT PROCESS as confirmed by examination of RISK MANAGEMENT FILE.....	See Appended RM Results Table 11.6.8	N/A
11.7	ME EQUIPMENT, ME SYSTEM, and ACCESSORIES coming into direct or indirect contact with biological tissues, cells, or body fluids assessed and documented per ISO 10993	No such parts.	N/A
11.8	Interruption and restoration of power supply did not result in a HAZARDOUS SITUATION, except interruption of its intended function	Shall be evaluated during end medical product approval. EUT is medical power supply unit intended for building-in.	N/A

12	ACCURACY OF CONTROLS AND INSTRUMENTS AND PROTECTION AGAINST HAZARDOUS OUTPUTS		N/A
12.1	RISKS associated with accuracy of controls and instruments stated in RISK MANAGEMENT PROCESS confirmed by RISK MANAGEMENT FILE review	See Appended RM Results Table 12.1	N/A
12.2	RISK of poor USABILITY, including identification, marking, and documents addressed in a USABILITY ENGINEERING PROCESS as confirmed by review of provided records.....	See Report based on IEC 60601-1-6	N/A
12.3	The need for alarm systems as a means of RISK CONTROL and RISKS associated with operation or failure of alarm system addressed in RISK MANAGEMENT PROCESS	See Report based on IEC 60601-1-8 and appended RM Results Table 12.3 No alarm incorporated.	N/A
12.4	Protection against hazardous output		N/A
12.4.1	RISKS associated with hazardous output arising from intentional exceeding of safety limits addressed in RISK MANAGEMENT PROCESS as confirmed in RISK MANAGEMENT FILE	See Appended RM Results Table 12.4.1	N/A
12.4.2	When applicable, need for indication of parameters associated with hazardous output addressed in RISK MANAGEMENT PROCESS as confirmed in RISK MANAGEMENT FILE	See Appended RM Results Table 12.4.2	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
12.4.3	RISKS associated with accidental selection of excessive output values for ME EQUIPMENT with a multi-purpose unit designed to provide low and high-intensity outputs for different treatments addressed in RISK MANAGEMENT PROCESS, confirmed in RISK MANAGEMENT FILE .. :	See Appended RM Results Table 12.4.3 Single output voltage.	N/A
12.4.4	When applicable, RISKS associated with incorrect output addressed in RISK MANAGEMENT PROCESS as confirmed by review of RISK MANAGEMENT FILE	See Appended RM Results Table 12.4.4	N/A
12.4.5	Diagnostic or therapeutic radiation		N/A
12.4.5.1	Adequate provisions to protect OPERATORS, PATIENTS, other persons and sensitive devices in vicinity of unwanted or excessive radiation emitted by ME EQUIPMENT designed to produce radiation for diagnostic/therapeutic purposes	--	N/A
	Radiation safety ensured by compliance with requirements of appropriate standards	--	N/A
12.4.5.2	RISKS associated with diagnostic X-rays addressed in RISK MANAGEMENT PROCESS as confirmed in RISK MANAGEMENT FILE..... :	See IEC 60601-1-3 Report and appended RM Results Table 12.4.5.2	N/A
12.4.5.3	RISKS associated with radiotherapy addressed in RISK MANAGEMENT PROCESS as confirmed by review of RISK MANAGEMENT FILE..... :	See Appended RM Results Table 12.4.5.3	N/A
12.4.5.4	RISKS associated with ME EQUIPMENT producing diagnostic or therapeutic radiation other than diagnostic X-rays and radiotherapy addressed in RISK MANAGEMENT PROCESS as confirmed by examination of RISK MANAGEMENT FILE..... :	See Appended RM Results Table 12.4.5.4	N/A
12.4.6	When applicable, RISKS associated with diagnostic or therapeutic acoustic pressure addressed in RISK MANAGEMENT PROCESS as confirmed in RISK MANAGEMENT FILE..... :	See Appended RM Results Table 12.4.6	N/A

13	HAZARDOUS SITUATIONS AND FAULT CONDITIONS		P
13.1	Specific HAZARDOUS SITUATIONS		P
13.1.1	None of HAZARDOUS SITUATIONS in 13.1.2-13.1.4, inclusive, occurred when SINGLE FAULT CONDITIONS applied, one at a time, as in 4.7 and 13.2	No hazardous situations occur during single fault testing.	P
13.1.2	Emissions, deformation of ENCLOSURE or exceeding maximum temperature		P
	– Emission of flames, molten metal, poisonous or ignitable substance in hazardous quantities did not occur	Not occur during single fault testing.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– Deformation of ENCLOSURE impairing compliance with 15.3.1 did not occur	No external enclosure provided. EUT is intended for building-in within end medical product.	N/A
	– Temperatures of APPLIED PARTS did not exceed allowable values in Table 24 when measured as in 11.1.3..... :	See appended Tables 11.1.1, 11.1.2.1, and 11.1.2.2 No applied parts provided.	N/A
	– Temperatures of ME EQUIPMENT parts that are not APPLIED PARTS likely to be touched did not exceed values in Table 23 when measured and adjusted as in 11.1.3..... :	See appended Tables 11.1.1, 11.1.2.1, and 11.1.2.2	P
	–Allowable values for “other components and materials” in Table 22 times 1.5 minus 12.5 °C were not exceeded	Considered.	P
	Limits for windings in Tables 26, 27, and 31 not exceeded	--	P
	Table 22 not exceeded in all other cases	--	P
	Temperatures measured according to 11.1.3	--	P
	SINGLE FAULT CONDITIONS in 4.7, 8.1 b), 8.7.2, and 13.2.2 relative to emission of flames, molten metal, or ignitable substances, not applied to parts and components where:	Single faults performed.	P
	– Supply circuit was unable to supply 15 W one minute after 15 W drawn from supply circuit, or	See appended Table 13.1.2	N/A
	– Parts and components completely contained within a fire ENCLOSURE complying with 11.3 as verified by review of design documentation	--	N/A
	After tests of this Clause, settings of THERMAL CUT-OUTS and OVER-CURRENT RELEASES did not change sufficiently to affect their safety function	--	N/A
13.1.3	– limits for LEAKAGE CURRENT in SINGLE FAULT CONDITION based on 8.7.3 did not exceed..... :	See appended Table 8.7	P
	– voltage limits for ACCESSIBLE PARTS including APPLIED PARTS in 8.4.2 did not exceed :	See appended Table 8.7 Output voltage.	P
13.1.4	ME EQUIPMENT complied with the requirements of 9.1 to 9.8 for specific MECHANICAL HAZARDS	--	P
13. 2	SINGLE FAULT CONDITIONS		P
13.2.1	During application of SINGLE FAULT CONDITIONS in 13.2.2 -13.2.13, inclusive, NORMAL CONDITIONS in 8.1 a) applied in least favourable combination :	See appended Table 13.2	P
13.2.2 – 13.2.12	ME EQUIPMENT complied with 13.2.2 -13.2.12..... :	See appended Table 13.2 and RM Results Table 13.2.6	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
13.2.13	ME EQUIPMENT remained safe after tests of 13.2.13.2 to 13.2.13.4 (inclusive), and cooling down to room temperature	No heating elements or motors provided. EUT is intended for continuous operation.	N/A
	ME EQUIPMENT examined for compliance or appropriate tests such as dielectric strength of motor insulation according to 8.8.3 conducted	--	N/A
	For insulation of thermoplastic materials relied upon as a MEANS OF PROTECTION (see 8.8), the ball-pressure test specified in 8.8.4.1 a) performed at a temperature 25 °C higher than temperature of insulation measured during tests of 13.2.13.2 to 13.2.13.4 (inclusive).	--	N/A
13.2.13.2	ME EQUIPMENT with heating elements		N/A
	a 1) thermostatically controlled ME EQUIPMENT with heating elements for building-in, or for unattended operation, or with a capacitor not protected by a fuse connected in parallel with THERMOSTAT contacts met tests of 13.2.13.2 b) & 13.2.13.2 c)	No heating elements provided.	N/A
	a 2) ME EQUIPMENT with heating elements RATED for non-CONTINUOUS OPERATION met tests of 13.2.13.2 b) and 13.2.13.2 c)	--	N/A
	a 3) other ME EQUIPMENT with heating elements met test of 13.2.13.2 b)	--	N/A
	When more than one test was applicable to same ME EQUIPMENT, tests performed consecutively	--	N/A
	Heating period stopped when a heating element or an intentionally weak part of a non-SELF-RESETTING THERMAL CUT-OUT ruptured, or current interrupted before THERMAL STABILITY without possibility of automatic restoration	--	N/A
	Test repeated on a second sample when interruption was due to rupture of a heating element or an intentionally weak part	--	N/A
	Both samples met 13.1.2, and open circuiting of a heating element or an intentionally weak part in second sample not considered a failure by itself	--	N/A
	b) ME EQUIPMENT with heating elements tested per 11.1 without adequate heat discharge, and supply voltage set at 90 or 110 % of RATED supply voltage, least favourable of the two (V) :	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Operating period stopped when a non-SELF-RESETTING THERMAL CUT-OUT operated, or current interrupted without possibility of automatic restoration before THERMAL STABILITY	--	N/A
	ME EQUIPMENT switched off as soon as THERMAL STABILITY established and allowed to cool to room temperature when current not interrupted	--	N/A
	Test duration was equal to RATED operating time for non-CONTINUOUS OPERATION	--	N/A
	c) Heating parts of ME EQUIPMENT tested with ME EQUIPMENT operated in NORMAL CONDITION at 110 % of RATED supply voltage and as in 11.1, and	--	N/A
	1) Controls limiting temperature in NORMAL CONDITION disabled, except THERMAL CUT-OUTS	--	N/A
	2) When more than one control provided, they were disabled in turn	--	N/A
	3) ME EQUIPMENT operated at RATED DUTY CYCLE until THERMAL STABILITY achieved, regardless of RATED operating time	--	N/A
13.2.13.3	ME EQUIPMENT with motors		N/A
	a 1) For the motor part of the ME EQUIPMENT, compliance checked by tests of 13.2.8- 13.2.10, 13.2.13.3 b), 13.2.13.3 c), and 13.2.13.4, as applicable	No motors provided.	N/A
	To determine compliance with 13.2.9 and 13.2.10 motors in circuits running at 42.4 V peak a.c./ 60 V d.c. or less are covered with a single layer of cheesecloth which did not ignite during the test	--	N/A
	a 2) Tests on ME EQUIPMENT containing heating parts conducted at prescribed voltage with motor & heating parts operated simultaneously to produce the least favourable condition	--	N/A
	a 3) Tests performed consecutively when more tests were applicable to the same ME EQUIPMENT	--	N/A
	b) Motor met running overload protection test of this clause when:	--	N/A
	1) it is intended to be remotely or automatically controlled by a single control device with no redundant protection, or	--	N/A
	2) it is likely to be subjected to CONTINUOUS OPERATION while unattended	--	N/A
	Motor winding temperature determined during each steady period and maximum value did not exceed Table 27 (Insulation Class, Maximum temperature measured °C)..... :	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Motor removed from ME EQUIPMENT and tested separately when load could not be changed in appropriate steps	--	N/A
	Running overload test for motors operating at 42.4 V peak a.c./60 V d.c. or less performed only when examination and review of design indicated possibility of an overload	--	N/A
	Test not conducted where electronic drive circuits maintained a substantially constant drive current	--	N/A
	Test not conducted based on other justifications (justification) :	--	N/A
	c) ME EQUIPMENT with 3-phase motors operated with normal load, connected to a 3-phase SUPPLY MAINS with one phase disconnected, and periods of operation per 13.2.10	--	N/A
13.2.13.4	ME EQUIPMENT RATED for NON-CONTINUOUS OPERATION		N/A
	ME EQUIPMENT (other than HAND-HELD) operated under normal load and at RATED voltage or at upper limit of RATED voltage range until increase in temperature was $\leq 5^{\circ}\text{C}$ in one hour, or a protective device operated	EUT is designed for continuous operation.	N/A
	When a load-reducing device operated in NORMAL USE, test continued with ME EQUIPMENT running idle	--	N/A
	Motor winding temperatures did not exceed values in 13.2.10..... :	--	N/A
	Insulation Class :	--	—
	Maximum temperature measured ($^{\circ}\text{C}$) :	--	—

14	PROGRAMMABLE ELECTRICAL MEDICAL SYSTEMS (PEMS)		N/A
14.1	Requirements of this clause not applied to PESS when it provided no BASIC SAFETY or ESSENTIAL PERFORMANCE, or	EUT is not programmable electrical medical system.	N/A
	- when application of ISO 14971 showed that failure of PESS does not lead to unacceptable RISK :	See Appended RM Results Table 14.1	N/A
	Every PROCESS has been followed throughout the PEMS DEVELOPMENT LIFE-CYCLE and a RECORD of PROCESS has been made available as confirmed by RISK MANAGEMENT FILE REVIEW and assessment of PROCESSES cited in this Clause	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	MANUFACTURER considered the need for additional RISK CONTROL measures when unable to follow all PROCESSES identified in Clause 14 for each constituent component of PEMS as confirmed by RISK MANAGEMENT FILE review and assessment of PROCESSES cited in this Clause	--	N/A
	Assessment of PROCESSES cited in this Clause made by internal audits	--	N/A
14.2	Documents produced from application of Clause 14 are maintained and form a part of RISK MANAGEMENT FILE in addition to RECORDS and documents required by ISO 14971 :	--	N/A
14.3	RISK MANAGEMENT plan required by 3.5 of ISO 14971 includes reference to PEMS VALIDATION plan	--	N/A
14.4	A PEMS DEVELOPMENT LIFE-CYCLE including a set of defined milestones has been documented	--	N/A
	At each milestone, activities to be completed, and VERIFICATION methods to be applied to activities have been defined	--	N/A
	Each activity including its inputs and outputs defined, and each milestone identifies RISK MANAGEMENT activities that must be completed before that milestone	--	N/A
	PEMS DEVELOPMENT LIFE-CYCLE tailored for a specific development by making plans detailing activities, milestones, and schedules	--	N/A
	PEMS DEVELOPMENT LIFE-CYCLE includes documentation requirements	--	N/A
14.5	A documented system for problem resolution within and between all phases and activities of PEMS DEVELOPMENT LIFE-CYCLE has been developed and maintained where appropriate	--	N/A
	Problem resolution system meets the prescribed criteria depending on type of product:	--	N/A
	– it is documented as a part of PEMS DEVELOPMENT LIFE-CYCLE	--	N/A
	– it allows reporting of potential or existing problems affecting BASIC SAFETY or ESSENTIAL PERFORMANCE	--	N/A
	– it includes an assessment of each problem for associated RISKS	--	N/A
	– it identifies criteria that must be met for the issue to be closed	--	N/A
	– it identifies the action to be taken to resolve each problem	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
14.6	RISK MANAGEMENT PROCESS		N/A
14.6.1	MANUFACTURER considered HAZARDS associated with software and hardware aspects of PEMS including NETWORK/DATA COUPLING, components of third-party origin, legacy subsystems when compiling list of known or foreseeable HAZARDS	See Appended RM Results Table 14.6.1	N/A
	In addition to the material in ISO 14971, Annex D, list of possible sources for HAZARDS associated with PEMS includes specified causes	--	N/A
	– failure of NETWORK/DATA COUPLING to provide characteristics necessary for PEMS to achieve its BASIC SAFETY OR ESSENTIAL PERFORMANCE	--	N/A
	– undesired feedback [physical and data] (such as unsolicited/ out of range/ inconsistent input or input from electromagnetic interference)	--	N/A
	– unavailable data	--	N/A
	– lack of integrity of data	--	N/A
	– incorrect data	--	N/A
	– incorrect timing of data	--	N/A
	– unintended interactions within & among PESS	--	N/A
	– unknown aspects or quality of third-party software	--	N/A
	– unknown aspects or quality of third-party PESS	--	N/A
	– lack of data security, particularly vulnerability to tampering, unintended interaction with other programs and viruses	--	N/A
14.6.2	Suitably validated tools and PROCEDURES assuring each RISK CONTROL measure reduces identified RISK(S) satisfactorily provided in addition to PEMS requirements in Clause 6.1 of ISO 14971	See Appended RM Results Table 14.6.2	N/A
14.7	A documented requirement specification for PEMS and each of its subsystems (e.g. for a PESS) which includes ESSENTIAL PERFORMANCE and RISK CONTROL measures implemented by that system or subsystem.....	See Appended RM Results Table 14.7	N/A
14.8	An architecture satisfying the requirement is specified for PEMS and each of subsystems.....	See Appended RM Results Table 14.8	N/A
	The architecture specification makes use of considers the specified items to reduce RISK to an acceptable level, where appropriate:	--	N/A
	a) COMPONENTS WITH HIGH-INTEGRITY CHARACTERISTICS	--	N/A
	b) fail-safe functions	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) redundancy	--	N/A
	d) diversity;	--	N/A
	e) partitioning of functionality	--	N/A
	f) defensive design potentially limiting hazardous effects by restricting available output power or by introducing means to limit travel of actuators	--	N/A
	g) allocation of RISK CONTROL measures to subsystems and components of PEMS	--	N/A
	h) failure modes of components and their effects;	--	N/A
	i) common cause failures	--	N/A
	j) systematic failures	--	N/A
	k) test interval duration and diagnostic coverage	--	N/A
	l) maintainability	--	N/A
	m) protection from reasonably foreseeable misuse	--	N/A
	n) NETWORK/DATA COUPLING specification, when applicable	--	N/A
14.9	Design is broken up into subsystems, each with a design and test specification where appropriate, and descriptive data on design environment included in RISK MANAGEMENT FILE :	See Appended RM Results Table 14.9	N/A
14.10	A VERIFICATION plan containing the specified information used to verify and document functions implementing BASIC SAFETY, ESSENTIAL PERFORMANCE, or RISK CONTROL measures :	See Appended RM Results Table 14.10	N/A
	– milestone(s) when VERIFICATION is to be performed for each function	--	N/A
	– selection and documentation of VERIFICATION strategies, activities, techniques, and appropriate level of independence of the personnel performing the VERIFICATION	--	N/A
	– selection and utilization of VERIFICATION tools	--	N/A
	– coverage criteria for VERIFICATION	--	N/A
14.11	A PEMS VALIDATION plan containing validation of BASIC SAFETY & ESSENTIAL PERFORMANCE and requiring checks for unintended functioning of PEMS to perform and document PEMS VALIDATION	See Appended RM Results Table 14.11	N/A
	The person with overall responsibility for PEMS VALIDATION is independent of design team, and no member of a design team is responsible for PEMS VALIDATION of their own design	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	All professional relationships of members of PEMS VALIDATION team with members of design team documented in RISK MANAGEMENT FILE providing methods & results of PEMS VALIDATION	--	N/A
14.12	Continued validity of previous design documentation assessed under a documented modification/change PROCEDURE	--	N/A
14.13	Technical description includes the following information when PEMS is to be connected to other equipment outside control of PEMS MANUFACTURER by NETWORK/DATA COUPLING..... :	See Appended RM Results Table 14.13	N/A
	a) characteristics of NETWORK/DATA COUPLING necessary for PEMS to achieve its INTENDED USE	--	N/A
	b) list of HAZARDOUS SITUATIONS resulting from a failure of NETWORK/DATA COUPLING to provide the specified characteristics	--	N/A
	c) instructions to RESPONSIBLE ORGANIZATION containing required information and warnings	--	N/A
	– connection of PEMS to a NETWORK/DATA COUPLING that includes other equipment could result in previously unidentified RISKS and RESPONSIBLE ORGANIZATION shall identify, analyze, and control such RISKS	--	N/A
	– subsequent changes to NETWORK/DATA COUPLING introducing new RISKS and requiring new analysis; and changes to NETWORK/DATA COUPLING include:	--	N/A
	– NETWORK/DATA COUPLING configuration change	--	N/A
	– connection of additional items to NETWORK/DATA COUPLING	--	N/A
	– disconnecting items from NETWORK/DATA COUPLING	--	N/A
	– update of equipment connected to NETWORK/DATA COUPLING	--	N/A
	– upgrade of equipment connected to NETWORK/DATA COUPLING	--	N/A
15	CONSTRUCTION OF ME EQUIPMENT		P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.1	RISKS associated with arrangement of controls and indicators of ME EQUIPMENT addressed in RISK MANAGEMENT PROCESS, as confirmed by examination of RISK MANAGEMENT FILE :	See Appended RM Results Table 15.1 The risk management requirements of the standard were not addressed. EUT is intended for building-in. There is only green indicator light to indicate power ON.	N/E
15.2	Parts of ME EQUIPMENT subject to mechanical wear, electrical, environmental degradation or ageing resulting in unacceptable RISK when unchecked for a long period, are accessible for inspection, replacement, and maintenance	No such parts provided.	N/A
	Inspection, servicing, replacement, and adjustment of parts of ME EQUIPMENT can easily be done without damage to or interference with adjacent parts or wiring	--	N/A
15.3	Mechanical strength		N/A
15.3.1	Mold stress relief, push, impact, drop, and rough handling tests did not result in unacceptable RISK and ME EQUIPMENT displayed adequate mechanical strength	EUT is intended for building-in and provided without external enclosure; therefore end product consideration.	N/A
15.3.2	Push test conducted by subjecting external parts of ENCLOSURE to a steady force of 250 N \pm 10 N for 5 s applied to a circular (30mm) plane surface, except bottom of ENCLOSURE of an ME EQUIPMENT >18 kg, using a suitable test tool ... :	See Appended Table 15.3 and RM Results Table 15.3.2	N/A
	No damage resulting in an unacceptable RISK sustained as determined by examination of RISK MANAGEMENT FILE	--	N/A
15.3.3	Impact test conducted by subjecting a complete ENCLOSURE or its largest non-reinforced area, except for HAND-HELD ME EQUIPMENT and parts, to a free falling 500 g \pm 25 g solid smooth steel ball, approx. 50 mm in diameter from a height of 1.3 m :	See Appended Table 15.3 and RM Results Table 15.3.3	N/A
	Test not applied to flat panel displays, platen glass of ME EQUIPMENT, or cathode ray tubes	--	N/A
	No damage resulting in an unacceptable RISK sustained as shown in RISK MANAGEMENT FILE	--	N/A
15.3.4	Drop test		N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.3.4.1	Sample of HAND-HELD ME EQUIPMENT and HAND-HELD part with SAFE WORKING LOAD allowed to fall freely once from each of 3 different positions as in NORMAL USE from height specified in ACCOMPANYING DOCUMENTS, or from 1 m onto a 50 mm \pm 5 mm thick hardwood board lying flat on a concrete or rigid base..... :	See Appended Table 15.3	N/A
	No unacceptable RISK resulted	--	N/A
15.3.4.2	Sample of PORTABLE ME EQUIPMENT and PORTABLE part with SAFE WORKING LOAD lifted to a height as in Table 29 above a 50 \pm 5 mm thick hardwood board lying flat on a concrete floor or rigid base, dropped 3 times from each orientation in NORMAL USE (cm) :	See Appended Table 15.3 and RM Table 15.3.4.2	N/A
	No damage resulting in an unacceptable RISK sustained as determined by examination of sample and RISK MANAGEMENT FILE	--	N/A
15.3.5	Each sample of MOBILE ME EQUIPMENT and MOBILE part with SAFE WORKING LOAD and in most adverse condition in NORMAL USE passed Rough Handling tests :	See Appended Table 15.3 and RM Results Table 15.3.5	N/A
	a) Ascending step shock test conducted on the sample by pushing it 3 times in its normal direction of travel at 0.4 m/s \pm 0.1 m/s against an ascending hardwood step obstruction without the sample going over the obstruction	--	N/A
	b) Descending step shock test conducted on the sample by pushing it 3 times in its normal direction of travel at 0.4 m/s \pm 0.1 m/s in order to fall over a vertical step affixed flat on a rigid base with direction of movement perpendicular to face of the step until full descent achieved	--	N/A
	c) Door frame shock test conducted on the sample by moving it 3 times in its normal direction of travel at 0.4 m/s \pm 0.1 m/s, or for motor driven EQUIPMENT, at maximum possible speed against a hardwood vertical obstacle higher than EQUIPMENT contact point(s)	--	N/A
	No damage resulting in an unacceptable RISK sustained as determined by examination of sample and RISK MANAGEMENT FILE	--	N/A
15.3.6	Examination of ENCLOSURE made from molded or formed thermoplastic material indicated that material distortion due to release of internal stresses by molding or forming operations will not result in an unacceptable RISK	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Mold-stress relief test conducted by placing one sample of complete ME EQUIPMENT, ENCLOSURE or a portion of larger ENCLOSURE, for 7 hours in a circulating air oven at 10°C over the max temperature measured on ENCLOSURE in 11.1.3, but no less than 70 °C :	--	N/A
	No damage resulting in an unacceptable RISK	--	N/A
15.3.7	INTENDED USE, EXPECTED SERVICE LIFE, and conditions for transport and storage were taken into consideration for selection and treatment of materials used in construction of ME EQUIPMENT	--	N/A
	Based on review of EQUIPMENT, ACCOMPANYING DOCUMENTS, specifications and processing of materials, and MANUFACTURER's relevant tests or calculations, corrosion, ageing, mechanical wear, degradation of biological materials due to bacteria, plants, animals and the like, will not result in an unacceptable RISK	--	N/A
15.4	ME EQUIPMENT components and general assembly		P
15.4.1	Incorrect connection of accessible connectors, removable without a TOOL, prevented where an unacceptable RISK exists, in particular :	See Appended RM Results Table 15.4.1 EUT is intended for building-in. End product consideration.	N/A
	a) Plugs for connection of PATIENT leads cannot be connected to other outlets on same ME EQUIPMENT intended for other functions, except when RISK MANAGEMENT FILE provides proof that no unacceptable RISK could result :	See attachment # No such plugs provided.	N/A
	b) Medical gas connections on ME EQUIPMENT for different gases to be operated in NORMAL USE are not interchangeable as verified by review of RISK MANAGEMENT FILE :	See attachment # No medical gas connections provided.	N/A
15.4.2	Temperature and overload control devices		P
15.4.2.1	a) THERMAL CUT-OUTS and OVER-CURRENT RELEASES with automatic resetting not used in ME EQUIPMENT when their use could result in a HAZARDOUS SITUATION by resetting action as verified by review of RISK MANAGEMENT FILE :	See Appended RM Results Table 15.4.2.1 a) No such components incorporated within the power supply unit.	N/A
	b) THERMAL CUT-OUTS with a safety function to be reset by a soldering operation affecting operating value not fitted in ME EQUIPMENT as verified by examination of design and RISK MANAGEMENT FILE :	See Appended RM Results Table 15.4.2.1 b) No such component used.	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	c) An independent non-SELF-RESETTING THERMAL CUT-OUT is, additionally, provided where a failure of a THERMOSTAT could constitute a HAZARD as verified by examination of design and RISK MANAGEMENT FILE..... :	See Appended RM Results Table 15.4.2.1 c) No thermostat provided.	N/A
	d) Based on design and RISK MANAGEMENT FILE review, loss of function of ME EQUIPMENT due to operation of THERMAL CUT-OUT or OVER CURRENT RELEASE doesn't result in a HAZARDOUS SITUATION	See Appended RM Results Table 15.4.2.1 d) EUT is not end medical product. The risk management requirements of the standard were not addressed. Shall be evaluated during end medical product approval.	N/E
	e) Capacitors or other spark-suppression devices not connected between contacts of THERMAL CUT-OUTS	--	N/A
	f) Use of THERMAL CUT-OUTS or OVER-CURRENT RELEASES do not affect safety of ME EQUIPMENT as verified by following tests:	--	P
	Positive temperature coefficient devices (PTC's) complied with IEC 60730-1: 1999, clauses 15, 17, J.15, and J.17 as applicable	--	N/A
	ME EQUIPMENT containing THERMAL CUT-OUTS and OVER-CURRENT RELEASES operated under the conditions of Clause 13..... :	See appended Table 13.2	P
	SELF-RESETTING THERMAL CUT-OUTS and OVER-CURRENT RELEASES including circuits performing equivalent functions (other than PTC's) Certified according to appropriate standards ..	--	N/A
	In the absence of Certification in accordance with IEC standards, SELF-RESETTING THERMAL CUT-OUTS and OVER-CURRENT RELEASES including circuits performing equivalent functions (other than PTC's) operated 200 times	--	N/A
	Manual reset THERMAL CUT-OUTS and OVER-CURRENT RELEASES Certified in accordance with appropriate IEC standards	No such components incorporated within the equipment.	N/A
	When certification based on IEC standards, or data from MANUFACTURER demonstrating reliability of component to perform its safety-related function is not available, manual reset THERMAL CUT-OUTS and OVER-CURRENT RELEASES operated 10 times	--	N/A
	Thermal protective devices tested separately from ME EQUIPMENT when engineering judgment indicated test results would not be impacted	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	g) Protective device, provided on ME EQUIPMENT incorporating a fluid filled container with heating means, operated when heater switched on with container empty and prevented an unacceptable RISK due to overheating	--	N/A
	h) ME EQUIPMENT with tubular heating elements provided with protection against overheating in both leads where a conductive connection to earth could result in overheating as verified by review of design and RISK MANAGEMENT FILE :	See Appended RM Results Table 15.4.2.1 h)	N/A
15.4.2.2	Temperature settings clearly indicated when means provided to vary setting of THERMOSTATS	No thermostats incorporated.	N/A
15.4.3	Batteries		N/A
15.4.3.1	Battery housings from which gases can escape during charging or discharging likely to result in a HAZARD ventilated to minimize RISK of accumulation and ignition as verified by review of design and RISK MANAGEMENT FILE :	See Appended RM Results Table 15.4.3.1 No batteries inside power supply unit provided. Mains operated equipment.	N/A
	Battery compartments prevent accidental short circuiting of battery when this could result in a HAZARDOUS SITUATION as verified by examination of design and RISK MANAGEMENT FILE	--	N/A
15.4.3.2	Means provided to prevent incorrect connection of polarity when a HAZARDOUS SITUATION may develop by incorrect connection or replacement of a battery :	See Appended RM Results Table 15.4.3.2	N/A
15.4.3.3	Overcharging of battery prevented by virtue of design when it could result in an unacceptable RISK as verified by review of design :	See Appended RM Results Table 15.4.3.3	N/A
15.4.3.4	Lithium batteries that could become a HAZARD complied with appropriate tests of IEC 60086-4	See Appended RM Results Table 15.4.3.4	N/A
	Tests of IEC 60086-4 waived on the lithium battery based on examination of design	--	N/A
15.4.3.5	A properly RATED protective device provided within INTERNAL ELECTRICAL POWER SOURCE to protect against fire caused by excessive currents when (in case of a short circuit) layout of internal wiring, cross-sectional area, rating of connected components can result in a fire :	See Appended RM Results Table 15.4.3.5	N/A
	Protective device has adequate breaking capacity to interrupt the maximum fault current	--	N/A
	Justification for OVER-CURRENT RELEASES or FUSE exclusion is included in RISK MANAGEMENT FILE	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.4.4	Indicator lights provided to indicate ME EQUIPMENT is ready for NORMAL USE, except when apparent to OPERATOR from normal operating position, and marking of 7.4.1 are insufficient for this purpose	See Appended RM Results Table 15.4.4 EUT is intended for building-in. End product consideration. The risk management requirements of the standard were not addressed.	N/E
	An additional indicator light provided on ME EQUIPMENT with a stand-by state or a warm-up state exceeding 15 s, except when apparent to OPERATOR from normal operating position	--	N/A
	Indicator lights provided on ME EQUIPMENT incorporating non-luminous heaters to indicate heaters are operational when a HAZARDOUS SITUATION could exist, except when apparent to OPERATOR from normal operating position	No heaters provided.	N/A
	Requirement not applied to heated stylus-pens for recording purposes	--	N/A
	Indicator lights provided on ME EQUIPMENT to indicate an output exists where an accidental or prolonged operation of output circuit could constitute a HAZARDOUS SITUATION	EUT is not end medical product. Shall be evaluated during end medical product approval.	N/A
	Colours of indicator lights complied with 7.8.1	--	N/A
	Charging mode visibly indicated in ME EQUIPMENT incorporating a means for charging an INTERNAL ELECTRICAL POWER SOURCE	No charging mode provided.	N/A
15.4.5	RISKS associated with pre-set controls addressed in RISK MANAGEMENT PROCESS when applicable as verified by review of RISK MANAGEMENT FILE	See Appended RM Results Table 15.4.5 No pre-set controls provided.	N/A
15.4.6	Actuating parts of controls of ME EQUIPMENT		N/A
15.4.6.1	a) Actuating parts cannot be pulled off or loosened up during NORMAL USE	No actuating parts of controls provided.	N/A
	b) Indication of scales (e.g., "on" "off" positions, etc.) always corresponds to position of controls with adjustment that can result in a HAZARDOUS SITUATION for PATIENT or OPERATOR while ME EQUIPMENT is in use	--	N/A
	c) Incorrect connection of indicating device to relevant component prevented by adequate construction when it could be separated without use of a TOOL	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	When torque values per Table 30 applied between control knob and shaft of rotating controls for not less than 2 s, 10 times in each direction, knobs did not rotate :	See appended Table 15.4.6	N/A
	Tests conducted by applying an axial force of 60 N for electrical components and 100 N for other components for 1 min when an axial pull was required in NORMAL USE with no unacceptable RISK :	See appended Table 15.4.6	N/A
15.4.6.2	Stops of adequate mechanical strength provided on rotating/ movable parts of controls of ME EQUIPMENT where necessary to prevent an unexpected change from max to min, or vice-versa, of the controlled parameter when this could cause a HAZARDOUS SITUATION :	See appended Table 15.4.6	N/A
	Torque values in Table 30 applied 10 times in each direction to rotating controls for 2 sec ... :	See appended Table 15.4.6	N/A
	Application of an axial force of 60 N for electrical components and 100 N for other components to rotating or movable parts of controls for 1 min when an axial pull was required in NORMAL USE :	See appended Table 15.4.6	N/A
15.4.7	Cord-connected HAND-HELD and foot-operated control devices		N/A
15.4.7.1	a) HAND-HELD control devices of ME EQUIPMENT complied with 15.3.4.1	EUT is not cord-connected hand-held or foot-operated control device.	N/A
	b) Foot-operated control device supported an actuating force of 1350 N for 1 min applied over an area of 30 mm diameter in its position of NORMAL USE with no damage to device causing an unacceptable RISK..... :	--	N/A
15.4.7.2	Control device of HAND-HELD and foot-operated control devices turned in all possible abnormal positions and placed on a flat surface :	--	N/A
	No unacceptable RISK caused by changing control setting when accidentally placed in an abnormal position	--	N/A
15.4.7.3	a) Foot-operated control device is at least IPX1 & complies with tests of IEC 60529 (IP Code) .. :	See appended Table 11.6	N/A
	b) ENCLOSURE of foot operated control devices containing electrical circuits is at least IPX6 and complies with IEC 60529 if in NORMAL USE liquids are likely to be found (IP Code) :	See appended Table 11.6 and RM Results Table 15.4.7.3 b)	N/A
	Probability of occurrence estimated as part of RISK MANAGEMENT PROCESS	--	N/A
15.4.8	Aluminum wires less than 16 mm ² in cross-sectional area are not used	Aluminium wires not used.	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.4.9	a) Oil container in PORTABLE ME EQUIPMENT allows for expansion of oil and is adequately sealed to prevent loss of oil in any position	--	N/A
	b) Oil containers in MOBILE ME EQUIPMENT sealed to prevent loss of oil during transport	--	N/A
	A pressure-release device operating during NORMAL USE is, optionally, provided	--	N/A
	c) Partially sealed oil-filled ME EQUIPMENT and its parts provided with means for checking the oil level to detect leakage	--	N/A
	ME EQUIPMENT and technical description examined, and manual tests conducted to confirm compliance with above requirements	--	N/A
15.5	MAINS SUPPLY TRANSFORMERS OF ME EQUIPMENT and transformers providing separation in accordance with 8.5		P
15.5.1	Overheating		P
15.5.1.1	Transformers of ME EQUIPMENT are protected against overheating in the event of short circuit or overload of output windings and comply with this Clause and tests of 15.5.1.2 – 3	See appended Tables 15.5.1.2 and 15.5.1.3	P
	During tests, windings did not open, no HAZARDOUS SITUATION occurred, and maximum temperatures of windings did not exceed values in Table 31	--	P
	Dielectric strength test of 8.8.3 conducted on transformer after short circuit and overload tests	See appended Table 15.5.2 No break-down of the insulation.	N/A
15.5.1.2	Transformer output winding short circuited, and test continued until protective device operated or THERMAL STABILITY achieved	See appended Table 15.5.1.2	P
	Short circuit applied directly across output windings for transformers not tested according to 5X frequency and 5X voltage test of 15.5.2	Short circuit performed on transformer secondary windings.	P
15.5.1.3	Multiple overload tests conducted on windings with more than one protective device to evaluate worst-case NORMAL USE loading and protection.....	See appended Table 15.5.1.3 Only one secondary winding.	N/A
15.5.2	Transformer windings provided with adequate insulation to prevent internal short-circuits that could cause overheating which could result in a HAZARDOUS SITUATION	--	P
	Dielectric strength tests were conducted in accordance with requirements of this clause with no breakdown of insulation system and no detectable deterioration of transformer	See appended Table 15.5.2	P

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.5.3	Transformers forming MEANS OF PROTECTION as required by 8.5 comply with IEC 61558-1:1997, Clause 5.12	See appended Table 8.10 Transformer tested within the equipment.	P
16	ME SYSTEMS		N/A
16.1	After installation or subsequent modification, ME SYSTEM didn't result in an unacceptable RISK	See Appended RM Results Table 16.1 EUT is a single components (intended for building-in) and therefore not treated as ME system.	N/A
	Only HAZARDS arising from combining various equipment to form a ME SYSTEM considered	--	N/A
	– ME SYSTEM provides the level of safety within the PATIENT ENVIRONMENT equivalent to ME EQUIPMENT complying with this standard	--	N/A
	– ME SYSTEM provides the level of safety outside PATIENT ENVIRONMENT equivalent to equipment complying with their respective IEC or ISO safety standards	--	N/A
	– tests performed in NORMAL CONDITION, except as specified	--	N/A
	– tests performed under operating conditions specified by MANUFACTURER of ME SYSTEM	--	N/A
	Safety tests previously conducted on individual equipment of ME SYSTEM according to relevant standards not repeated	--	N/A
	RISK MANAGEMENT methods, optionally, used by MANUFACTURER of an ME SYSTEM reconfigurable by RESPONSIBLE ORGANIZATION or OPERATOR to determine configurations with highest RISKS and measures to ensure any configuration of ME SYSTEM will not present unacceptable RISKS	--	N/A
	Non-ME EQUIPMENT used in ME SYSTEM complied with applicable IEC or ISO safety standards	--	N/A
	Equipment relying only on BASIC INSULATION for protection against electric shock not used in ME SYSTEM	--	N/A
16.2	ACCOMPANYING DOCUMENTS of an ME SYSTEM		N/A
	Documents containing all data necessary for ME SYSTEM to be used as intended by MANUFACTURER including a contact address accompany ME SYSTEM or modified ME SYSTEM	--	N/A
	ACCOMPANYING DOCUMENTS regarded as a part of ME SYSTEM	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	ACCOMPANYING DOCUMENTS are, optionally, provided in electronic format (e.g. electronic file format or CD ROM) and ME SYSTEM is capable of displaying or printing these documents	--	N/A
	a) ACCOMPANYING DOCUMENTS provided for each item of ME EQUIPMENT supplied by MANUFACTURER	--	N/A
	b) ACCOMPANYING DOCUMENTS provided for each item of non-ME EQUIPMENT supplied by MANUFACTURER	--	N/A
	c) the required information is provided:	--	N/A
	– specifications, instructions for use as intended by MANUFACTURER, and a list of all items forming the ME SYSTEM	--	N/A
	– instructions for installation, assembly, and modification of ME SYSTEM to ensure continued compliance with this standard	--	N/A
	– instructions for cleaning and, when applicable, disinfecting and sterilizing each item of equipment or equipment part forming part of the ME SYSTEM	--	N/A
	– additional safety measures to be applied during installation of ME SYSTEM	--	N/A
	– identification of parts of ME SYSTEM suitable for use within the PATIENT ENVIRONMENT	--	N/A
	– additional measures to be applied during preventive maintenance	--	N/A
	– a warning forbidding placement of MULTIPLE SOCKET-OUTLET, when provided and it is a separate item, on the floor	--	N/A
	– a warning indicating an additional MULTIPLE SOCKET-OUTLET or extension cord not to be connected to ME SYSTEM	--	N/A
	– a warning to connect only items that have been specified as part of ME SYSTEM or specified as being compatible with ME SYSTEM	--	N/A
	– maximum permissible load for any MULTIPLE SOCKET-OUTLET(S) used with ME SYSTEM	--	N/A
	– instructions indicating MULTIPLE SOCKET-OUTLETS provided with the ME SYSTEM to be used only for supplying power to equipment intended to form part of ME SYSTEM	--	N/A
	– an explanation indicating RISKS of connecting non-ME EQUIPMENT supplied as a part of ME SYSTEM directly to wall outlet when non-ME EQUIPMENT is intended to be supplied via a MULTIPLE SOCKET-OUTLET with a separating transformer	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– an explanation indicating RISKS of connecting any equipment supplied as a part of ME SYSTEM to MULTIPLE SOCKET-OUTLET	--	N/A
	– permissible environmental conditions of use for ME SYSTEM including conditions for transport and storage	--	N/A
	– instructions to OPERATOR not to, simultaneously, touch parts referred to in 16.4 and PATIENT	--	N/A
	d) the following instructions provided for use by RESPONSIBLE ORGANIZATION:	--	N/A
	– adjustment, cleaning, sterilization, and disinfection PROCEDURES	--	N/A
	– assembly of ME SYSTEMS and modifications during actual service life shall be evaluated based on the requirements of this standard	--	N/A
16.3	Instructions for use of ME EQUIPMENT intended to receive its power from other equipment in an ME SYSTEM, describe the other equipment to ensure compliance with these requirements	--	N/A
16.4	Parts of non-ME EQUIPMENT in PATIENT ENVIRONMENT subject to contact by OPERATOR during maintenance, calibration, after removal of covers, connectors, etc., without use of a TOOL operated at a voltage \leq voltage in 8.4.2 c) supplied from a source separated from SUPPLY MAINS by two MEANS OF OPERATOR PROTECTION	--	N/A
16.5	Safety measures incorporating a SEPARATION DEVICE applied when FUNCTIONAL CONNECTION between ME EQUIPMENT and other items of an ME SYSTEM or other systems can cause allowable values of LEAKAGE CURRENT to exceed	--	N/A
	SEPARATION DEVICE has dielectric strength, CREEPAGE and CLEARANCES required for one MEANS OF OPERATOR PROTECTION appropriate for highest voltage occurring across SEPARATION DEVICE during a fault condition	--	N/A
	WORKING VOLTAGE was highest voltage across SEPARATION DEVICE during a fault condition, but not less than MAXIMUM MAINS VOLTAGE (V)..... :	--	N/A
16.6	LEAKAGE CURRENTS		N/A
16.6.1	TOUCH CURRENT in NORMAL CONDITION, from or between parts of ME SYSTEM within the PATIENT ENVIRONMENT, did not exceed 100 μ A :	See appended Table 16.6.1	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	TOUCH CURRENT did not exceed 500 μ A in event of interruption of any non-PERMANENTLY INSTALLED PROTECTIVE EARTH CONDUCTOR, from or between parts of ME SYSTEM within PATIENT ENVIRONMENT	See appended Table 16.6.1	N/A
16.6.2	Current in PROTECTIVE EARTH CONDUCTOR of MULTIPLE SOCKET-OUTLET did not exceed 5 mA..:	--	N/A
16.6.3	PATIENT LEAKAGE CURRENT and total PATIENT LEAKAGE CURRENT of ME SYSTEM in NORMAL CONDITION did not exceed values specified for ME EQUIPMENT in Tables 3 and 4	See appended Tables 8.7 8.7.4.7 and 16.6.1	N/A
	Measurements made using a device as in clause 8.7.4.4	--	N/A
16.7	ME SYSTEM complied with applicable requirements of Clause 9 when a MECHANICAL HAZARD existed	See applicable appended Tables in section 9	N/A
16.8	Interruption and restoration of relevant power connections of ME SYSTEM one at a time and all connections simultaneously did not result in a HAZARDOUS SITUATION other than interruption of its intended function	--	N/A
16.9	ME SYSTEM connections and wiring		N/A
16.9.1	Incorrect connection of accessible connectors, removable without a TOOL, prevented where a HAZARDOUS SITUATION could otherwise exist.....:	See Appended RM Results Table 16.9.1	N/A
	– Connectors complied with Clause 15.4.1	--	N/A
	– Plugs for connection of PATIENT leads could not be connected to other outlets of the same ME SYSTEM likely to be located in PATIENT ENVIRONMENT, except when examination of connectors and interchanging them proved no HAZARDOUS SITUATION could result	--	N/A
16.9.2	MAINS PARTS, components and layout	--	N/A
16.9.2.1	a) – MULTIPLE SOCKET-OUTLET only allows connection using a TOOL, or	--	N/A
	– MULTIPLE SOCKET-OUTLET is of a type that cannot accept MAINS PLUGS of any of the kinds specified in IEC/TR 60083, or	--	N/A
	– MULTIPLE SOCKET-OUTLET is supplied via a separating transformer	--	N/A
	b) – MULTIPLE SOCKET-OUTLET marked with safety sign 2 of Table D.2 (i.e., safety sign ISO 7010-W001) visible in NORMAL USE, and	--	N/A
	– marked either individually or in combinations, with the maximum allowed continuous output in amperes or volt-amperes, or	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– marked to indicate the equipment or equipment parts it may safely be attached to	--	N/A
	– MULTIPLE SOCKET-OUTLET is a separate item or an integral part of ME EQUIPMENT or non-ME EQUIPMENT	--	N/A
	c) MULTIPLE SOCKET-OUTLET complied with IEC 60884-1 and the following requirements:	--	N/A
	– CREEPAGE and CLEARANCES complied with 8.9	--	N/A
	– It is CLASS I, and PROTECTIVE EARTH CONDUCTOR is connected to earthing contacts in socket-outlets	--	N/A
	– PROTECTIVE EARTH TERMINALS and PROTECTIVE EARTH CONNECTIONS comply with 8.6, except total impedance for ME SYSTEM was up to 400 mΩ, or higher when conditions of 8.6.4 b) met (mΩ).. :	--	N/A
	– ENCLOSURE complied with 8.4.2 d)	--	N/A
	– MAINS TERMINAL DEVICES and wiring complied with 8.11.4, when applicable	--	N/A
	– RATINGS of components are not in conflict with conditions of use	See appended Table 8.10	N/A
	– Electrical terminals and connectors of MULTIPLE SOCKET-OUTLETS prevent incorrect connection of accessible connectors removable without a TOOL	--	N/A
	– POWER SUPPLY CORD complied with 8.11.3	--	N/A
	d) Additional requirements applied when MULTIPLE SOCKET-OUTLET combined with a separating transformer:	--	N/A
	– Separating transformer complied with IEC 61558-2-1, except requirements of maximum RATED output power of 1 kVA and degree of protection IPX4 were not applied	See appended Table 8.10	N/A
	– Separating transformer is CLASS I	--	N/A
	– Degree of protection against ingress of water specified as in IEC 60529	--	N/A
	– Separating transformer assembly marked according to 7.2 and 7.3	--	N/A
	– MULTIPLE SOCKET-OUTLET permanently connected to separating transformer, or socket-outlet of separating transformer assembly cannot accept MAINS PLUGS as identified in IEC/TR 60083	--	N/A
16.9.2.2	Removal of any single item of equipment in ME SYSTEM will not interrupt the protective earthing of any other part without simultaneous disconnection of electrical supply to that part	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Additional PROTECTIVE EARTH CONDUCTORS can be detachable only by use of a TOOL	--	N/A
16.9.2.3	Conductors connecting different items within an ME SYSTEM protected against mechanical damage	--	N/A

17	ELECTROMAGNETIC COMPATIBILITY OF ME EQUIPMENT AND ME SYSTEMS		N/E
	RISKS associated with items addressed in RISK MANAGEMENT PROCESS as confirmed by review .:	See Appended RM Results Table 17 The risk management requirements of the standard were not addressed. Electromagnetic compatibility shall be evaluated during end medical product approval.	N/E
	– electromagnetic phenomena at locations where ME EQUIPMENT or ME SYSTEM is to be used as stated in ACCOMPANYING DOCUMENTS.....:	--	N/E
	– introduction of electromagnetic phenomena into environment by ME EQUIPMENT or ME SYSTEM that might degrade performance of other devices, electrical equipment, and systems	--	N/E

ANNEX G	PROTECTION AGAINST HAZARDS OF IGNITION OF FLAMMABLE ANESTHETIC MIXTURES		N/A
G.2	Locations and basic requirements		N/A
G.2.1	Parts of CATEGORY APG ME EQUIPMENT in which a FLAMMABLE ANESTHETIC MIXTURE WITH AIR occurs are CATEGORY AP or APG ME EQUIPMENT and complied with G.3, G.4, and G.5	EUT was not tested against hazard of ignition of flammable anaesthetic mixtures.	N/A
G.2.2	FLAMMABLE AESTHETIC MIXTURE WITH AIR occurring due to a leakage or discharge of a FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN or NITROUS OXIDE from an ENCLOSURE considered 5 to 25 cm from point of occurrence	--	N/A
G.2.3	A FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN or NITROUS OXIDE contained in a completely / partly enclosed ME EQUIPMENT part and in PATIENT'S respiratory tract 5 cm from an ENCLOSURE part where leakage or discharge occurs	--	N/A
G.2.4	ME EQUIPMENT or parts thereof specified for use with FLAMMABLE AESTHETIC MIXTURE WITH AIR (in a location as in G.2.2) are CATEGORY AP or APG ME EQUIPMENT and complied with G.4 and G.5	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
G.2.5	ME EQUIPMENT or parts thereof for use with FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN OR NITROUS OXIDE (location per G.2.2) are CATEGORY APG ME EQUIPMENT and comply with G.4 and G.6	--	N/A
	ME EQUIPMENT in G.2.3 to G.2.5 met appropriate tests of G.3-G.5 conducted after tests of 11.6.6 and 11.6.7	--	N/A
G.3	Marking, ACCOMPANYING DOCUMENTS		N/A
G.3.1	CATEGORY APG ME EQUIPMENT prominently marked. With a green-coloured band ≥ 2 cm wide with letters "APG" according to symbol 23 in Table D.1..... :	See copies of Marking Labels	N/A
	Length of green-coloured band is ≥ 4 cm, and size of marking is as large as possible for particular case	--	N/A
	When above marking not possible, relevant information included in instructions for use ... :	--	N/A
	Marking complied with tests and criteria of 7.1.2 and 7.1.3	--	N/A
G.3.2	CATEGORY AP ME EQUIPMENT prominently marked, with a green-coloured circle ≥ 2 cm in diameter, with characters "AP" according to symbol 22 in Table D.1..... :	See copies of Marking Labels	N/A
	Marking is as large as possible for the particular case	--	N/A
	When above marking not possible, the relevant information included in instructions for use ... :	--	N/A
	Marking complied with tests and criteria of 7.1.2 and 7.1.3	--	N/A
G.3.3	The marking according to G.3.2 and G.3.3 placed on major part of ME EQUIPMENT for CATEGORY AP or APG parts, and not repeated on detachable parts that can only be used with the marked EQUIPMENT	--	N/A
G.3.4	ACCOMPANYING DOCUMENTS contain an indication enabling the RESPONSIBLE ORGANIZATION to distinguish between CATEGORY AP and APG parts	--	N/A
G.3.5	Marking clearly indicates which parts are CATEGORY AP or APG when only certain ME EQUIPMENT parts are CATEGORY AP or APG	--	N/A
G.4	Common requirements for CATEGORY AP and CATEGORY APG ME EQUIPMENT		N/A
G.4.1	a) CREEPAGE and CLEARANCES between points of POWER SUPPLY CORD connection are according to Table 12 for one MEANS OF PATIENT PROTECTION	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	b) Connections, except those in circuits described in G.5.3 and G.6.3, protected against accidental disconnection in NORMAL USE or connection and disconnection can be performed only with a TOOL	--	N/A
	c) CATEGORY AP and APG not provided with a DETACHABLE POWER SUPPLY CORD, except when circuit complied with G.5.3 and G.6.3	--	N/A
G.4.2	Construction details		N/A
	a) Opening of an ENCLOSURE providing protection against penetration of gases or vapours into ME EQUIPMENT or its parts possible only with a TOOL	--	N/A
	b) ENCLOSURE complies with requirements to minimize arcing and sparking due to penetration of foreign objects	See appended Table 8.10	N/A
	– no openings on top covers of ENCLOSURE, except for openings for controls covered by control knobs	--	N/A
	– openings in side-covers prevented penetration of a solid cylindrical test rod of 4 mm in diameter applied in all possible directions without appreciable force	--	N/A
	– openings in base plates prevented penetration of a solid cylindrical test rod of 12 mm in diameter applied in all directions without appreciable force	--	N/A
	c) Short circuiting conductor(s) to a conductive part without presence of explosive gasses where insulation may contact a part containing a FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN or NITROUS OXIDE, ignitable gases alone, or oxygen, did not result in loss of integrity of the part, an unacceptable temperature, or other HAZARD	--	N/A
G.4.3	a) Electrostatic charges prevented on CATEGORY AP and APG ME EQUIPMENT by a combination of appropriate measures	--	N/A
	– Use of antistatic materials with a limited electrical resistance as specified in G.4.3 b) ...:	See appended Table 8.10	N/A
	– Provision of electrically conductive paths from ME EQUIPMENT or its parts to a conductive floor, protective earth or potential equalization system, or via wheels to an antistatic floor of medical room	--	N/A
	b) Electrical resistance limits of aesthetic tubing, mattresses and pads, castor tires, and other antistatic material complied with ISO 2882 based on measurements according to ISO 1853, ISO 2878 and ISO 23529	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
G.4.4	Corona cannot be produced by components or parts of ME EQUIPMENT operating at more than 2000 V a.c. or 2400 V d.c. and not included in ENCLOSURES complying with G.5.4 or G.5.5	--	N/A
G.5	Requirements and tests for CATEGORY AP ME EQUIPMENT, parts and components		N/A
G.5.1	ME EQUIPMENT, its parts or components do not ignite FLAMMABLE AESTHETIC MIXTURES WITH AIR under NORMAL USE and CONDITIONS based on compliance with G.5.2 to G.5.5 (inclusive)	--	N/A
	Alternatively, ME EQUIPMENT, its parts, and components complied with requirements of IEC 60079-0 for pressurized ENCLOSURES (IEC 60079-2); for sand-filled ENCLOSURES, IEC 60079-5; or for oil immersed equipment, IEC 60079-6; and with this standard excluding G.5.2 to G.5.5 :	--	N/A
G.5.2	ME EQUIPMENT, its parts, and components in contact with gas mixtures in NORMAL USE and CONDITIONS not producing sparks and not resulting in surface temperatures above 150 °C in case of restricted or 200 °C in case of unrestricted vertical air circulation measured at 25 °C comply with G.5.1 :	See appended Tables 11.1.1, 11.1.2.1, 11.1.2.2, & 11.2.2.1	N/A
G.5.3	ME EQUIPMENT, its parts, and components producing sparks in NORMAL USE and CONDITION complied with temperature requirements of G.5.2, and U_{max} and I_{max} occurring in their circuits, and complied as follows:	--	N/A
	Measured $U_{max} \leq U_{zR}$ with I_{zR} as in Fig. G.1 :	--	N/A
	Measured $U_{max} \leq U_c$ with C_{max} as in Fig. G.2 ... :	--	N/A
	Measured $I_{max} \leq I_{zR}$ with U_{zR} as in Fig G.1 :	--	N/A
	Measured $I_{max} \leq I_{zL}$ with L_{max} and a $U_{max} \leq 24 V$ as in Fig G.3 :	--	N/A
	– Combinations of currents and corresponding voltages within the limitations $I_{zR}.U_{zR} \leq 50 W$ extrapolated from Fig G.1	--	N/A
	No extrapolation made for voltages above 42 V	--	N/A
	– Combinations of capacitances and corresponding voltages within limitations of $C/2U^2 \leq 1.2 mJ$ extrapolated from Fig G.2	--	N/A
	No extrapolation made for voltages above 242V	--	N/A
	U_{max} , additionally, determined using actual resistance R when the equivalent resistance R was less than 8000 Ω	--	N/A
	– Combinations of currents and corresponding inductances within limitations $L/2I^2 \leq 0.3 mJ$ extrapolated from Fig G.3	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	No extrapolation made for inductances larger than 900 mH	--	N/A
	– U_{max} was the highest supply voltage occurring in circuit under investigation with sparking contact open, taking into consideration MAINS VOLTAGE variations in 4.10	--	N/A
	– I_{max} was the highest current flowing in circuit under investigation with sparking contact closed, taking into consideration MAINS VOLTAGE variations required in 4.10	--	N/A
	– C_{max} and L_{max} taken as values occurring at the component under investigation producing sparks	--	N/A
	– Peak value considered when a.c. supplied	--	N/A
	– An equivalent circuit calculated to determine equivalent max capacitance, inductance, and equivalent U_{max} and I_{max} , either as d.c. or a.c. peak values in case of a complicated circuit... :	--	N/A
	Temperature measurements made according to 11.1, and U_{max} , I_{max} , R , L_{max} , and C_{max} determined with application of Figs G.1-G.3... :	See appended Tables 11.1.1, 11.1.2.1, & 11.1.2.2	N/A
	Alternatively, compliance was verified by examination of design data..... :	--	N/A
G.5.4	External ventilation with internal overpressure		N/A
	ME EQUIPMENT, its parts, and components enclosed in an ENCLOSURE with external ventilation by means of internal overpressure complied with the following requirements:	--	N/A
	a) FLAMMABLE AESTHETIC MIXTURES WITH AIR that might have penetrated into ENCLOSURE of ME EQUIPMENT or part removed by ventilation before EQUIPMENT energized, and penetration of such mixtures during operation was prevented by maintenance of overpressure by means of air without flammable gases, or by physiologically acceptable inert gas (e.g., nitrogen)	--	N/A
	b) Overpressure inside ENCLOSURE was 75 Pa, min., in NORMAL CONDITION (Pa) :	--	N/A
	Overpressure maintained at the site of potential ignition even when air or inert gas could escape through openings in ENCLOSURE necessary for normal operation of ME EQUIPMENT or its parts	--	N/A
	ME EQUIPMENT could be energized only after the required minimum overpressure was present long enough to ventilate the ENCLOSURE so that the displaced volume of air or inert gas was at least five times the volume of ENCLOSURE	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	ME EQUIPMENT energized at will or repeatedly when overpressure was continuously present	--	N/A
	c) Ignition sources de-energized automatically by means used where G.4 does not apply, or complied with G.5 when during operation overpressure dropped below 50 Pa (Pa) :	--	N/A
	d) External surface of ENCLOSURE in which internal overpressure was maintained did not exceed 150 °C in 25 °C ambient under NORMAL USE and CONDITION (°C) :	--	N/A
G.5.5	ENCLOSURES with restricted breathing		N/A
	ME EQUIPMENT, its parts, and components enclosed in an ENCLOSURE with restricted breathing complied with the following:	--	N/A
	a) A FLAMMABLE AESTHETIC MIXTURE WITH AIR did not form inside ENCLOSURE with restricted breathing when it was surrounded by a FLAMMABLE AESTHETIC MIXTURE WITH AIR of a high concentration for at least 30 min without any pressure difference inside ENCLOSURE	--	N/A
	b) Gasket or sealing material used to maintain tightness complied with aging test B-b of IEC 60068-2-2, Clause 15, at 70 °C ± 2 °C and 96 h :	See appended Table 8.10	N/A
	c) Gas-tightness of ENCLOSURE containing inlets for flexible cords maintained when the cords were stressed by bending or pulling	--	N/A
	Cords are fitted with adequate anchorages to limit stresses	--	N/A
	After the test in G.5.4 b), an internal overpressure of 400 Pa was created and 30 pulls of the value in Table G.1 applied to each flexible cord in axial direction of cord inlet and in the least favourable direction for 1 s	--	N/A
	Overpressure not reduced below 200 Pa	--	N/A
	Tests waived when examination of ENCLOSURE indicated it is completely sealed or gas-tight without a doubt (100 % degree of certainty)	--	N/A
	Operating temperature of external surface of ENCLOSURE was ≤ 150 °C in 25 °C (°C) :	--	N/A
	Steady state operating temperature of ENCLOSURE also measured (°C) :	--	N/A
G.6	CATEGORY APG ME EQUIPMENT, parts and components thereof		N/A
G.6.1	ME EQUIPMENT, its parts, and components did not ignite FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN OR NITROUS OXIDE under NORMAL USE and SINGLE FAULT CONDITION	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	ME EQUIPMENT, its parts, and components not complying with G.6.3 subjected to a CONTINUOUS OPERATION test after attaining thermal steady state (max. 3 h) over a period of 10 min in a 12.2 % \pm 0.4 ether by volume/oxygen mixture	--	N/A
G.6.2	Parts and components of CATEGORY APG ME EQUIPMENT operating in a FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN OR NITROUS OXIDE supplied from a source isolated from earth by insulation equal to one MEANS OF PATIENT PROTECTION and from electrical parts by insulation twice the MEANS OF PATIENT PROTECTION	--	N/A
G.6.3	Test of G.6.1 waived when the following requirements were met in NORMAL USE and under NORMAL and SINGLE FAULT CONDITIONS	--	N/A
	a) no sparks produced and temperatures did not exceed 90 °C, or	See Tables 11.1.1, 11.1.2.1, 11.1.2.2, 11.2.2.1, and 13.2	N/A
	b) a temperature limit of 90 °C not exceeded, sparks produced in NORMAL USE, and SINGLE FAULT CONDITIONS, except U_{max} and I_{max} occurring in their circuits complied with requirements, taking C_{max} and L_{max} into consideration:	See Tables 11.1.1, 11.1.2.1, 11.1.2.2, and 13.2	N/A
	Measured $U_{max} \leq U_{zR}$ with I_{zR} as in Fig. G.4	--	N/A
	Measured $U_{max} \leq U_{zC}$ with C_{max} as in Fig. G.5 ...	--	N/A
	Measured $I_{max} \leq I_{zR}$ with U_{zR} as in Fig G.4	--	N/A
	Measured $I_{max} \leq I_{zL}$ with L_{max} and a $U_{max} \leq 24$ V as in Fig G.6	--	N/A
	– Extrapolation from Figs G.4, G.5, and G.6 was limited to areas indicated	--	N/A
	– U_{max} was the highest no-load voltage occurring in the circuit under investigation, taking into consideration mains voltage variations as in 4.10	--	N/A
	– I_{max} was the highest current flowing in the circuit under investigation, taking into account MAINS VOLTAGE variations as in 4.10	--	N/A
	– C_{max} and L_{max} are values occurring in relevant circuit	--	N/A
	– U_{max} additionally determined with actual resistance R when equivalent resistance R in Fig G.5 was less than 8000 Ω	--	N/A
	– Peak value taken into consideration when a.c. supplied	--	N/A
	– An equivalent circuit calculated to determine max capacitance, inductance, and U_{max} and I_{max} , either as d.c. or a.c. peak values in case of a complicated circuit	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	– When energy produced in an inductance or capacitance in a circuit is limited by voltage or current-limiting devices, two independent components applied, to obtain the required limitation even when a first fault (short or open circuit) in one of these components	--	N/A
	Above requirement not applied to transformers complying with this standard	--	N/A
	Above requirement not applied to wire-wound current-limiting resistors provided with a protection against unwinding of the wire in case of rupture	--	N/A
	Compliance verified by examination of CATEGORY APG ME EQUIPMENT, parts, and components , or	--	N/A
	Temperature measurements made in accordance with 11.1, or	See Tables 11.1.1, 11.1.2.1, and 11.1.2.2	N/A
	U_{max} , I_{max} , R , L_{max} and C_{max} determined together with application of Figs G.4-G.6..... :	--	N/A
	Alternatively, compliance verified by comparison with design data:	--	N/A
G.6.4	ME EQUIPMENT, its parts, and components heating a FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN OR NITROUS OXIDE provided with a non-SELF-RESETTING THERMAL CUT-OUT and complied with 15.4.2.1..... :	See appended Table 8.10	N/A
	Current-carrying part of heating element is not in direct contact with FLAMMABLE AESTHETIC MIXTURE WITH OXYGEN OR NITROUS OXIDE	--	N/A
G.7	Test apparatus for flammable mixtures		N/A
	Test apparatus used was in accordance with this Clause and Fig G.7	--	N/A

ANNEX L	INSULATED WINDING WIRES FOR USE WITHOUT INTERLEAVED INSULATION		P
L.1	BASIC, SUPPLEMENTARY, DOUBLE, and REINFORCED INSULATION in wound components without interleaved insulation complied with this Annex covering round winding wires between 0.05 mm and 5.00 mm diameters	Approved triple insulated wire used for secondary windings of the transformer. See list of critical components for details.	P
L.2	Wire construction		N/A
	Overlap of layers when wire is insulated with two or more spirally wrapped layers of tape is adequate to ensure continued overlap during manufacture of wound component	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Layers of spirally wrapped wire insulation are sufficiently secured to maintain the overlap	--	N/A
L.3	Type Test		N/A
	The wire subjected to tests of L.3.1 to L.3.4 at a temperature and a relative humidity specified	--	N/A
	Temperature (°C)..... :	--	—
	Humidity (%) :	--	—
L.3.1	Dielectric strength		N/A
	Dielectric strength test of Clause 8.8.3 for the appropriate type and number of MOP(s) conducted by preparing the sample according to IEC 60851-5:1996, Clause 4.4.1 for a twisted pair with test voltages at least twice Tables 6 & 7, but not less than below with no breakdown:	--	N/A
	– 3000 V for BASIC and SUPPLEMENTARY INSULATION (V) :	--	N/A
	– 6000 V for REINFORCED INSULATION (V)..... :	--	N/A
L.3.2	Flexibility and adherence		N/A
	Sample subjected to flexibility and adherence test 8 of IEC 60851-3:1996, clause 5.1.1, using mandrel diameters of Table L.1	--	N/A
	Sample examined according to IEC 60851-3: 1997, clause 5.1.1.4, followed by dielectric test of clause 8.8.3, except test voltage applied between wire and mandrel with no breakdown	--	N/A
	Test voltage was at least the voltage in Tables 6 and 7 but not less than the following:	--	N/A
	– 1500 V for BASIC and SUPPLEMENTARY INSULATION (V) :	--	N/A
	– 3000 V for REINFORCED INSULATION (V) :	--	N/A
	Tension applied to wire during winding on mandrel calculated from the wire diameter equivalent to 118 Mpa ± 11.8 Mpa :	--	N/A
L.3.3	Heat Shock		N/A
	Sample subjected to heat shock test 9 of IEC 60851-6:1996, followed by dielectric strength test of clause 8.8.3, except test voltage applied between the wire and mandrel	--	N/A
	Test voltage was at least the voltage in Tables 6 and 7, but not less than the following:	--	N/A
	– 1500 V for BASIC and SUPPLEMENTARY INSULATION (V) :	--	N/A
	– 3000 V for REINFORCED INSULATION (V) :	--	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Oven temperature based on Table L.2 (°C)..... :	--	—
	Mandrel diameter and tension applied as in clause L.3.2, (Mpa; N/mm ²) :	--	N/A
	Dielectric strength test conducted at room temperature after removal from the oven	--	N/A
L.3.4	Retention of electric strength after bending		N/A
	Five samples prepared as in L.3.2 subjected to dielectric strength and bending tests	--	N/A
	Test voltage was at least the voltage in Tables 6 and 7, but not less than the following:	--	N/A
	– 1500 V for BASIC and SUPPLEMENTARY INSULATION (V)..... :	--	N/A
	– 3000 V for REINFORCED INSULATION (V) :	--	N/A
	Test voltage applied between the shot and conductor.	--	N/A
	Mandrel diameter and tension applied as in L.3.2, (Mpa; N/mm ²) :	--	N/A
L.4	Tests during manufacture		N/A
L.4.1	Production line dielectric strength tests conducted by the manufacture according to L.4.2 and L.4.3 :	See attached manufacturer's routine testing verification	N/A
L.4.2	Test voltage for routine testing (100 % testing) is at least the voltage in Tables 6 and 7 but not less than the following:	--	N/A
	– 1500 V r.m.s. or 2100 V peak for BASIC and SUPPLEMENTARY INSULATION (V)..... :	See manufacturer's routine testing verification	N/A
	– 3000 V r.m.s. or 4200 V peak for REINFORCED INSULATION (V) :	See manufacturer's routine testing verification	N/A
L.4.3	Sampling tests conducted using twisted pair samples (IEC 60851-5:1996, clause 4.4.1)	See manufacturer's routine testing verification	N/A
	Minimum breakdown test voltage at least twice the voltage in Tables 6 and 7 but not less than:	--	N/A
	– 3000 V r.m.s. or 4200 V peak for BASIC and SUPPLEMENTARY INSULATION	See manufacturer's routine testing verification	N/A
	– 6000 V r.m.s. or 8400 V peak for REINFORCED INSULATION	See manufacturer's routine testing verification	N/A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

4.2	RM RESULTS TABLE: Risk Management Process for ME Equipment or ME Systems		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
3.3a			
3.5e			
4.1			
4.2			
4.3			
4.4			
5			
6.1			
6.2			
6.3			
6.4			
6.5			
6.6			
6.7			
7			

Supplementary Information:

The risk management requirements of the standard were not addressed. EUT is intended for building-in and therefore not end medical product. All clauses required checking of RMF shall be evaluated during end medical product approval.

4.3	TABLE: ESSENTIAL PERFORMANCE		N/E
List of ESSENTIAL PERFORMANCE functions	MANUFACTURER'S document number reference or reference from this standard or collateral or particular standard(s)	Remarks	
Reinforced insulation between primary and secondary (2 x MOOP)	--	Tested in accordance with IEC60601-1: 2005 to comply with 2 x MOOP requirements.	
Reinforced insulation between primary and functional earth (2 x MOOP)	--	Tested in accordance with IEC60601-1: 2005 to comply with 2 x MOOP requirements.	
Basic insulation between primary and protective earth (1 x MOOP)	--	Tested in accordance with IEC60601-1: 2005 to comply with 1 x MOOP requirements.	

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
4.3	TABLE: ESSENTIAL PERFORMANCE		N/E
List of ESSENTIAL PERFORMANCE functions	MANUFACTURER'S document number reference or reference from this standard or collateral or particular standard(s)	Remarks	
Supplementary Information: The risk management requirements of the standard were not addressed. EUT is intended for building-in and therefore not end medical product. All clauses required checking of RMF shall be evaluated during end medical product approval. Essential performance is performance, the absence or degradation of which, would result in an unacceptable risk. Unacceptable risk would occur in case of MOOP isolation break-down or degradation.			

4.3	RM RESULTS TABLE: Essential Performance		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
<p>Supplementary Information:</p> <p>The risk management requirements of the standard were not addressed. EUT is intended for building-in and therefore not end medical product. All clauses required checking of RMF shall be evaluated during end medical product approval.</p>			

4.5	RM RESULTS TABLE: Equivalent Safety for ME Equipment of ME System		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
<p>Supplementary Information:</p> <p>The risk management requirements of the standard were not addressed.</p>			

4.6	RM RESULTS TABLE: ME Equipment or system parts contacting the patient		N/A
-----	---	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			

Supplementary Information:

No parts that can come into contact with the patient. No applied parts provided. EUT is intended for building-in.

4.7	RM RESULTS TABLE: Single Fault Condition for ME Equipment		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			

Supplementary Information:

The risk management requirements of the standard were not addressed. All applicable single fault conditions performed according to the standard.

4.8	RM RESULTS TABLE: Components of ME Equipment		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			

Supplementary Information:

IEC approved components provided within the unit. The risk management requirements of the standard were not addressed.

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

4.9	RM RESULTS TABLE: Use of components with high-integrity characteristics		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			

Supplementary Information:

Approved optocouplers and Y1 capacitors provided between primary and secondary circuit.

4.11	TABLE: Power Input					P
Operating Conditions / Ratings		Voltage (V)	Frequency (Hz)	Current (mA)	Power (VA/W)	Power factor (cos φ)
Model: GTM2065-553.3-FA						
Rated output load (3,3 Vdc / 16,67 A)		90	50	0,91	45,3/82,5	--
Rated output load (3,3 Vdc / 16,67 A)		100	50	0,85	44,8/84,9	--
Rated output load (3,3 Vdc / 16,67 A)		240	50	0,42	44,8/102,2	--
Rated output load (3,3 Vdc / 16,67 A)		264	50	0,40	45,6/104,7	--
Rated output load (3,3 Vdc / 16,67 A)		90	60	0,94	45,3/85,3	--
Rated output load (3,3 Vdc / 16,67 A)		100	60	0,86	44,9/86,5	--
Rated output load (3,3 Vdc / 16,67 A)		240	60	0,42	44,8/101,3	--
Rated output load (3,3 Vdc / 16,67 A)		264	60	0,39	45,7/103,7	--
Model: GTM2065-8048-FA						
Rated output load (48,0 Vdc / 1,67 A)		90	50	1,44	78,6/130,2	--
Rated output load (48,0 Vdc / 1,67 A)		100	50	1,32	77,6/132,3	--
Rated output load (48,0 Vdc / 1,67 A)		240	50	0,68	76,2/163,2	--
Rated output load (48,0 Vdc / 1,67 A)		264	50	0,64	77,6/168,9	--
Rated output load (48,0 Vdc / 1,67 A)		90	60	1,46	78,6/131,9	--
Rated output load (48,0 Vdc / 1,67 A)		100	60	1,33	77,6/133,4	--

IEC 60601-1						
Clause	Requirement + Test			Result - Remark		Verdict
4.11	TABLE: Power Input					P
Operating Conditions / Ratings		Voltage (V)	Frequency (Hz)	Current (mA)	Power (VA/W)	Power factor (cos φ)
Rated output load (48,0 Vdc / 1,67 A)		240	60	0,68	76,1/162,7	--
Rated output load (48,0 Vdc / 1,67 A)		264	60	0,63	77,7/167,8	--
Supplementary Information: See copy of marking plate for details.						

5.1	RM RESULTS TABLE: Type Tests		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary Information: /			

5.4 a)	RM RESULTS TABLE: Other Conditions		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary Information:			
Maximum ambient temperature: 50°C (specified by the manufacturer) for models with air flow rated 10 CFM, placed on the transformer (T1) side of the supply, so the direction of the air flow was towards the transformer T1 as specified by the manufacturer.			
Maximum ambient temperature: 45°C (specified by the manufacturer) for models without air flow.			
The risk management requirements of the standard were not addressed.			

5.7	RM RESULTS TABLE: Humidity preconditioning treatment			N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks		Verdict
4.2				
4.3				
4.4				
5				
6.2				

IEC 60601-1			
Clause	Requirement + Test		Verdict
5.7	RM RESULTS TABLE: Humidity preconditioning treatment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
6.3			
6.4			
6.5			
Supplementary Information: Standard humidity treatment performed.			

5.9.2	TABLE: Determination of ACCESSIBLE parts		N/A
Location		Determination method (NOTE1)	Comments
Supplementary information:			
NOTE 1 - The determination methods are: visual; rigid test finger; jointed test finger; test hook.			
Power supply unit is intended for building and provided without external enclosure. End product consideration.			

5.9.2.3	RM RESULTS TABLE: Actuating mechanisms		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary Information: No such parts. EUT is power supply unit intended for building-in within end medical product.			

7.1.2	TABLE: Legibility of Marking		N/A
Markings tested	Ambient illuminance (lx)	Remarks	
Outside Markings (Clause 7.2)	--	Marking plate	
Inside Markings (Clause 7.3)	--	No markings to be read inside	
Controls & Instruments (Clause 7.4)	--	No controls & instruments	

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
7.1.2	TABLE: Legibility of Marking		N/A
Safety Signs (Clause 7.5)	--	No safety signs	
Symbols (Clause 7.6).....	--	Present on Marking plate	
Supplementary information: Observer, with a visual acuity of 0 on the log Minimum Angle of Resolution (log MAR) scale or 6/6 (20/20), reads marking at ambient illuminance least favourable level in the range of 100 lx to 1,500 lx. The ME EQUIPMENT or its part was positioned so that the viewpoint was the intended position of the OPERATOR at any point within the base of a cone subtended by an angle of 30° to the axis normal to the centre of the plane of the marking and at a distance of 1 m.			
Supplementary Information: Power supply unit is intended for building-in. Marking plate provided on the balk capacitor. Marking plate shall not be visible from the outside after installation of the power supply unit within the end medical product. End product consideration.			

7.1.3	TABLE: Durability of marking test		P
Characteristics of the Marking Label tested:		Remarks	
Material of Marking Label	Foil sticker	Pass	
Ink/other printing material or process.....	Laser printing	Pass	
Material (composition) of Warning Label	--	N/A	
Ink/other printing material or process.....	--	N/A	
Other	--	N/A	
Supplementary information:			
Marking rubbed by hand, first for 15 s with a cloth rag soaked with distilled water, then for 15 s with a cloth rag soaked with methylated spirit, and then for 15 s with a cloth rag soaked with isopropyl alcohol.			
Supplementary Information:			
Marking plate provided on the balk capacitor. Marking plate shall not be visible from the outside after installation of the power supply unit within the end medical product due the fact that power supply unit is intended for building-in.			

7.2.2	RM RESULTS TABLE: Identification		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.4			
Supplementary Information: The risk management requirements of the standard were not addressed. Power supply unit is intended for building-in. End product consideration.			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
7.2.5	RM RESULTS TABLE: ME EQUIPMENT powered from other equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.4			
Supplementary Information: Mains operated equipment. EUT not supplied from other equipment.			

7.2.13	RM RESULTS TABLE: Physiological effects (safety signs and warning)		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.3			
Supplementary Information: EUT not produces physiological effects.			

7.2.17	RM RESULTS TABLE: Protective packaging		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.3			
6.4			
Supplementary Information: Protective packing not part of the investigation. EUT is power supply unit intended for building-in.			

7.3.3	RM RESULTS TABLE: Batteries		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict

IEC 60601-1			
Clause	Requirement + Test		Verdict
7.3.3	RM RESULTS TABLE: Batteries		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.3			
Supplementary Information: No batteries inside. Mains operated equipment.			

7.3.7	RM RESULTS TABLE: Supply terminals		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
Supplementary Information: Standard input / output connectors provided.			

7.4.2	RM RESULTS TABLE: Control devices		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
Supplementary Information: No control devices provided.			

7.5	RM RESULTS TABLE: Safety signs		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
7.5	RM RESULTS TABLE: Safety signs		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
6.3			
Supplementary Information: No safety signs provided. EUT is not end medical product.			

7.9.1	RM RESULTS TABLE: General accompanying documents (See Table C.4)		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
Supplementary Information: Paper version of accompanying documents provided by the manufacturer.			

7.9.2.4	RM RESULTS TABLE: Electrical power source		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.3			
Supplementary Information: No additional power source incorporated. Mains operated equipment.			

7.9.3.2	RM RESULTS TABLE: Replacement of fuses, power supply cords, other parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
7.9.3.2	RM RESULTS TABLE: Replacement of fuses, power supply cords, other parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
6.2			
6.3			
6.4			
6.5			
Supplementary Information: EUT is not permanently installed equipment.			

8.1 b(1)	RM RESULTS TABLE: Fundamental rule of protection against electric shock - interruption of any one power-carrying conductor		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
Supplementary Information: No conductor between ME equipment parts and separate enclosures.			

8.1 b(2)	RM RESULTS TABLE: Fundamental rule of protection against electric shock - unintended movement of a component		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary Information: All internal components are mounted securely to prevent excessive bending (Reduction of creepage and clearance distances prevented by design). Some internal components additionally fixed with glue. See enclosed pictures of the unit for details.			

8.1 b(3)	RM RESULTS TABLE: Fundamental rule of protection against electric shock - accidental detachment of conductors and connectors		N/A
----------	--	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.3			
Supplementary Information: There is only PE conductor connected between JZA and JZB (through the hole method in addition to soldering). See enclosed pictures of the unit for details.			

8.2.2	RM RESULTS TABLE: Connection to an external d.c. power sources		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary Information: Mains operated equipment. EUT not intended for connection to DC power source.			

8.3 d	RM RESULTS TABLE: Requirements of Type BF or CF Applied Parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.2		See also RM Table for 4.6	
Supplementary Information: No applied parts provided.			

8.4.2	TABLE: TABLE: Working Voltage / Power Measurement					P
Test supply voltage/frequency (V/Hz) ¹					264 Vac / 50 Hz	
Location From/To	Measured values					Remarks
	Vrms	Vpk or Vdc	Peak-to-peak ripple ²	Power W/VA	Energy (J)	
Model: GTM2065-333.3-F						
Measured between output minus and output plus	--	3,3 Vdc	--	62,7 VA	--	Maximum output current achieved: 19,0 A
Model: GTM2065-6548-F						
Measured between output minus and output plus	--	44,9 Vdc	--	121,3 VA	--	Maximum output current achieved: 2,7 A

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.4.2	TABLE: TABLE: Working Voltage / Power Measurement		P
Supplementary Information: 1. The input supply voltage to the ME EQUIPMENT shall be the RATED voltage or the voltage within the RATED voltage range which results in the highest measured value. See clause 8.5.4. 2. If the d.c peak-to-peak ripple >10%, waveform considered as a.c. See clause 8.4.2.2 Power supply unit is intended for building-in.			

8.4.2 c	RM RESULTS TABLE: Accessible parts including applied parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary Information: Power supply unit is intended for building-in. End product consideration.			

8.4.3	TABLE: ME EQUIPMENT for connection to a power source by a plug - measurement of voltage or calculation of stored charge 1 s after disconnection of plug from mains supply									P
Maximum allowable voltage (V)									60	
Voltage measured (V)										
Voltage Measured Between:	1	2	3	4	5	6	7	8	9	10
Plug pins 1 and 2	0	16	--	--	--	--	--	--	--	--
Plug pin 1 and plug earth pin	--	--	--	--	--	--	--	--	--	--
Plug pin 2 and plug earth pin	--	--	--	--	--	--	--	--	--	--
Plug pin 1 and enclosure	--	--	--	--	--	--	--	--	--	--
Plug pin 2 and enclosure	--	--	--	--	--	--	--	--	--	--
Maximum allowable stored charge when measured voltage exceeded 60 v (μc)									45	
Calculated stored charge (μc)										
Voltage Measured Between:	1	2	3	4	5	6	7	8	9	10
Plug pins 1 and 2										
Plug pin 1 and plug earth pin										
Plug pin 2 and plug earth pin										
Plug pin 1 and enclosure										
Plug pin 2 and enclosure										

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

Supplementary information:

Supply voltage: 264 Vac / 50 Hz

8.4.4	TABLE: Internal capacitive circuits – measurement of residual voltage or calculation of the stored charge in capacitive circuits (i.e., accessible capacitors or circuit parts) after de-energizing ME EQUIPMENT			N/A
Maximum allowable residual voltage (V):				60 V
Maximum allowable stored charge when residual voltage exceeded 60 V :				45 μC
Description of the capacitive circuit (i.e., accessible capacitor or circuit parts)	Measured residual voltage (V)	Calculated stored charge (μC)	Remarks	
Supplementary information: /				

8.5.2.2	RM RESULTS TABLE: Type B applied parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary Information:			
No applied parts provided. EUT is power supply unit intended for building-in.			

8.5.2.3	RM RESULTS TABLE: PATIENT Leads		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary Information:			
No patient leads provided.			

8.5.5.1a	TABLE: defibrillation-proof applied parts – measurement of hazardous electrical energies				N/A
Test Condition: Figs. 9 & 10	Measurement made on accessible part	Applied part with test voltage	Test voltage polarity	Measured voltage between Y1 and Y2 (mV)	Remarks

IEC 60601-1					
Clause	Requirement + Test			Result - Remark	Verdict
Supplementary information:					
No applied parts provided.					

8.5.5.1b	TABLE: defibrillation-proof applied parts – verification of recovery time				N/A
Applied part with test voltage	Test voltage polarity	Recovery time from documents (s)	Measured recovery time (s)	Remarks	
Supplementary information:					
No applied parts provided.					

8.5.5.2	TABLE: DEFIBRILLATION-PROOF APPLIED PARTS or PATIENT CONNECTIONS of DEFIBRILLATION-PROOF APPLIED PARTS - Energy reduction test –measurement of Energy delivered to a 100 Ω load			N/A
Test Voltage applied to		Measured Energy E1 (mJ)	Measured Energy E2 (mJ)	Energy E1 as % of E2 (%)
PATIENT CONNECTION 1 or APPLIED PART with PATIENT CONNECTIONS 2, 3, and 4 of the same APPLIED PART connected to earth				
PATIENT CONNECTION 2 or APPLIED PART with PATIENT CONNECTIONS 1, 3, and 4 of the same APPLIED PART connected to earth				
PATIENT CONNECTION 3 or APPLIED PART with PATIENT CONNECTIONS 1, 2, and 4 of the same APPLIED PART connected to earth				
PATIENT CONNECTION 4 or APPLIED PART with PATIENT CONNECTIONS 1, 2, and 3 of the same APPLIED PART connected to earth				
Supplementary information: For compliance: E1 must at least 90% of E2 E1= Measured energy delivered to 100 Ω with ME Equipment connected; E2= Measured energy delivered to 100 Ω without ME equipment connected.				
Supplementary Information:				
No applied parts provided.				


8.6.3	RM RESULTS TABLE: Protective earthing of moving parts			N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks		Verdict
4.2				
4.3				
4.4				
5				

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.6.3	RM RESULTS TABLE: Protective earthing of moving parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.2			
6.3			
6.4			
6.5			
Supplementary Information: No moving parts provided.			

8.6.4	TABLE: Impedance and current-carrying capability of PROTECTIVE EARTH CONNECTIONS				P
Type of ME EQUIPMENT & impedance measured between parts		Test current (A) /Duration (s)	Voltage drop measured between parts (V)	Maximum calculated impedance (mΩ)	Maximum allowable impedance (mΩ)
PERMANENTLY INSTALLED ME EQUIPMENT, impedance between PROTECTIVE EARTH TERMINAL and a PROTECTIVELY EARTHED part		--	--	--	100
Impedance between earth pin and a PROTECTIVELY EARTHED internal PE connection. See supplementary information below.		25 A / 1 min.			100
Impedance between earth pin and a PROTECTIVELY EARTHED internal PE connection. See supplementary information below.		40 A / 2 min.			100
ME EQUIPMENT with a non-DETACHABLE POWER SUPPLY CORD, impedance between the protective earth pin in the MAINS PLUG and a PROTECTIVELY EARTHED part		--	--	--	200
Supplementary information: Power supply unit is intended for building-in. PE conductor provided between JZA and JZB. Functional insulation provided between primary circuit and metal shield (reinforced insulation provided between those two parts). Measured between point A and point B marked on the picture on the next page.					

IEC 60601-1

Clause	Requirement + Test	Result - Remark	Verdict
--------	--------------------	-----------------	---------

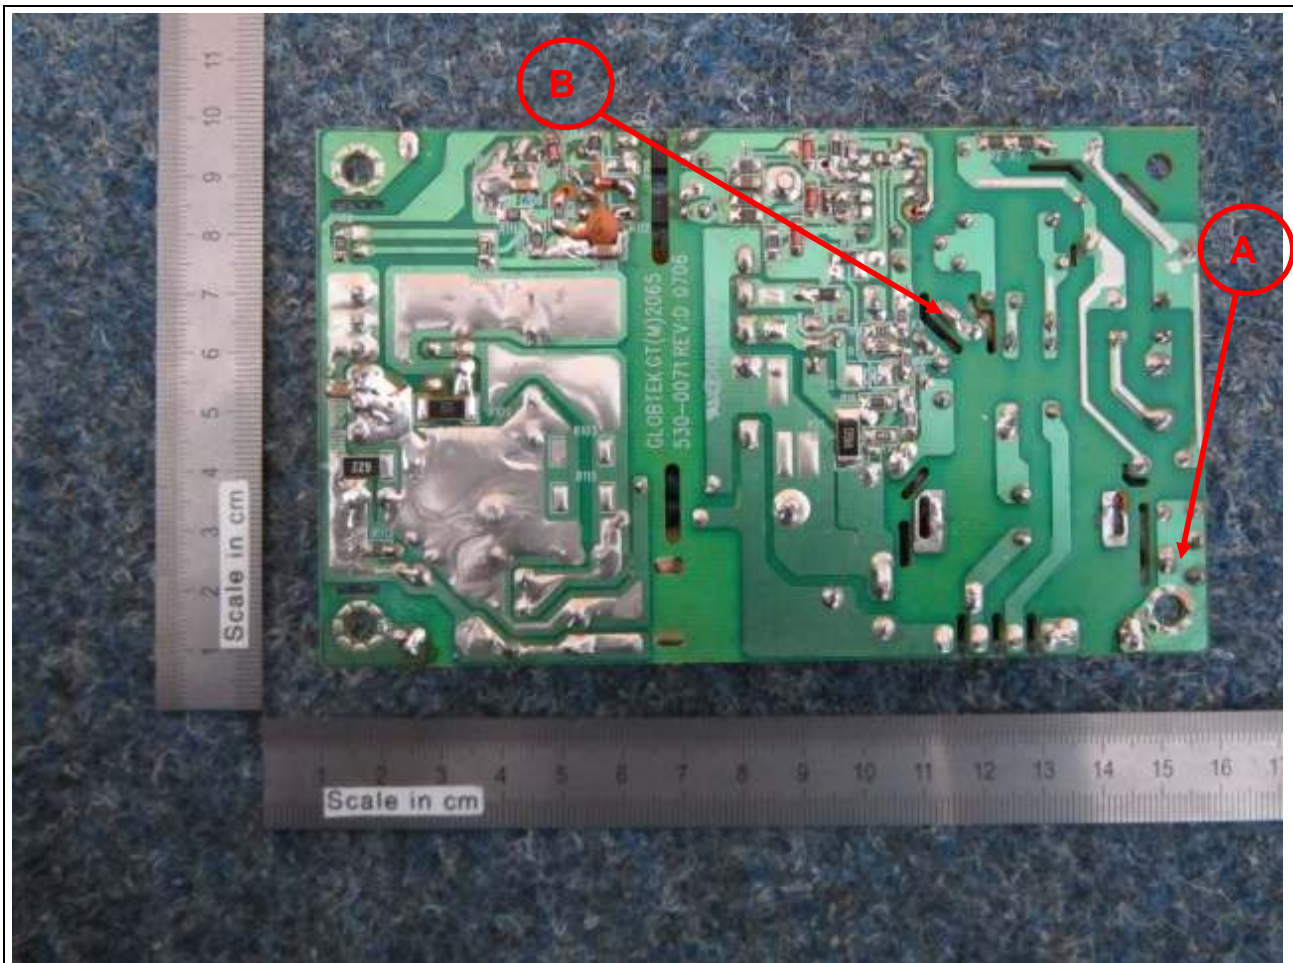

8.7	TABLE: leakage current			P
Type of leakage current and test condition (including single faults)	Supply voltage (V)	Supply frequency (Hz)	Measured max. value (μA)	Remarks
Fig. 13 - Earth Leakage (ER)	—	—	—	Maximum allowed values: 5 mA NC; 10 mA SFC
Normal condition, normal polarity, before humidity treatment	264	60	225,6	--
Normal condition, reverse polarity, before humidity treatment	264	60	222,8	--
Single fault condition (supply interruption), normal polarity, before humidity treatment	264	60	441,5	--
Single fault condition (supply interruption), reverse polarity, before humidity treatment	264	60	441,7	--

IEC 60601-1				
Clause	Requirement + Test		Result - Remark	
Normal condition, normal polarity, after humidity treatment	264	60	229,8	--
Normal condition, reverse polarity, after humidity treatment	264	60	227,6	--
Single fault condition (supply interruption), normal polarity, after humidity treatment	264	60	445,6	--
Single fault condition (supply interruption), reverse polarity, after humidity treatment	264	60	445,5	--
Fig. 14 - Touch Current (TC)	—	—	—	Maximum allowed values: 100 uA NC; 500 uA SFC
Normal condition, normal polarity, before humidity treatment	264	60	84,2	Measured on output
Normal condition, reverse polarity, before humidity treatment	264	60	84,2	Measured on output
Single fault condition (supply interruption), normal polarity, before humidity treatment	264	60	133,7	Measured on output
Single fault condition (supply interruption), reverse polarity, before humidity treatment	264	60	133,7	Measured on output
Single fault condition (PE interruption), normal polarity, before humidity treatment	264	60	40,2	Measured on output
Single fault condition (PE interruption), reverse polarity, before humidity treatment	264	60	39,8	Measured on output
Normal condition, normal polarity, after humidity treatment	264	60	88,5	Measured on output
Normal condition, reverse polarity, after humidity treatment	264	60	88,4	Measured on output
Single fault condition (supply interruption), normal polarity, after humidity treatment	264	60	137,2	Measured on output
Single fault condition (supply interruption), reverse polarity, after humidity treatment	264	60	137,1	Measured on output
Single fault condition (PE interruption), normal polarity, after humidity treatment	264	60	42,6	Measured on output
Single fault condition (PE interruption), reverse polarity, after humidity treatment	264	60	40,7	Measured on output

IEC 60601-1				
Clause	Requirement + Test		Result - Remark	Verdict
Fig. 15 - Patient Leakage Current (P)	—	—	—	Maximum allowed values: Type B or BF AP: 10 uA NC; 50 uA SFC (d.c. current); 100 uA NC; 500 uA SFC (a.c.) Type CF AP: 10 uA NC; 50 uA SFC (d.c. or a.c. current)
Fig. 16 - Patient leakage current with mains on the F-type applied parts (PM)	—	—	—	Maximum allowed values: Type B: N/A Type BF AP: 5000 uA Type CF AP: 50 uA
Fig. 17 - Patient leakage current with external voltage on Signal Input/Output part (SIP/SOP)	—	—	—	Maximum allowed values: Type B or BF AP: 10 uA NC; 50 uA SFC(d.c. current); 100 uA NC; 500 uA SFC (a.c.) ; Type CF AP: 10 uA NC; 50 uA SFC (d.c. or a.c. current)
Fig. 18 - Patient leakage current with external voltage on metal Accessible Part that is not Protectively Earthed	—	—	—	Maximum allowed values: Type B or BF AP: 500 uA Type CF: N/A
Fig. 19 – Patient Auxiliary Current	—	—	—	Maximum allowed values: Type B or BF AP: 10 uA NC; 50 uA SFC (d.c. current); 100 uA NC; 500 uA SFC (a.c.) ; Type CF AP: 10 uA NC;50 uA SFC (d.c. or a.c. current)
Fig. 15 and 20 – Total Patient Leakage Current with all AP of same type connected together	—	—	—	Maximum allowed values: Type B or BF AP: 50 uA NC; 100uA SFC (d.c. current); 500 uA NC; 1000 uA SFC (a.c.); Type CF AP: 50 uA NC; 100 uA SFC (d.c. or a.c. current)
Fig. 17 and 20 – Total Patient Leakage Current with all AP of same type connected together with external voltage on SIP/SOP	—	—	—	Maximum allowed values: Type B or BF AP: 50 uA NC; 100uA SFC (d.c. current); 500 uA NC;1000 uA SFC (a.c.); Type CF AP: 50 uA NC; 100 uA SFC (d.c. or a.c. current)

IEC 60601-1				
Clause	Requirement + Test		Result - Remark	Verdict
Fig. 16 and 20 – Total Patient Leakage Current with all AP of same type connected together with external voltage on F-type AP	—	—	—	Maximum allowed values: Type B: NA Type BF: 5000uA Type CF: 100 uA
Fig. 18 and 20 – Total Patient Leakage Current with all AP of same type connected together with external voltage on metal Accessible Part not Protectively Earthed	—	—	—	Maximum allowed values: Type B & BF: 1000 uA Type CF: N/A
<p>Note 1: For EARTH LEAKAGE CURRENT see 8.7.3 d) and 8.7.4.5; Note 2: For TOUCH CURRENT see 8.7.3 c) and 8.7.4.6; Note 3: For PATIENT LEAKAGE CURRENT SEE 8.7.3.b) and 8.7.4.7 Note 4: Total PATIENT LEAKAGE CURRENT values are only relative to equipment with multiple APPLIED PARTS of the same type. See 8.7.4.7 h). The individual APPLIED PARTS complied with the PATIENT LEAKAGE CURRENT values. Note 5: In addition to conditions indicated in the Table, tests conducted at operating temperature and after humidity preconditioning of 5.7, EQUIPMENT energized in stand-by condition and fully operating, max rated supply frequency, at 110 % of the max RATED MAINS VOLTAGE, and after relevant tests of Clause 11.6 (i.e., overflow, spillage, leakage, ingress of water and particulate matter, cleaning & disinfection, & sterilization).</p>				
<p>ER - Earth leakage current TC – Touch current P - Patient leakage current PA – Patient auxiliary current TP – Total Patient current PM - Patient leakage current with mains on the applied parts MD - Measuring device</p> <p>A - After humidity conditioning B - Before humidity conditioning 1 - Switch closed or set to normal polarity 0 - Switch open or set to reversed polarity NC - Normal condition SFC - Single fault condition</p>				
<p>Supplementary information:</p> <p>Leakage current measured with metal PE shield installed as in normal use (metal shield is separated from mains by reinforced insulation).</p> <p>CY3= CY4= 470 pF CY1= CY2= CY5= CY6= 1000 pF CY7= CY8= 470 pF</p>				

8.8.3	TABLE: Dielectric strength test of solid insulating materials with safety function – MEANS OF OPERATOR PROTECTION (MOOP) / MEANS OF PATIENT PROTECTION (MOPP)				P
Insulation under test (area from insulation diagram)	Insulation Type (1 or 2 MOOP/MOPP)	Reference Voltage		A.C. test voltages in V r.m.s ¹	Dielectric breakdown after 1 minute Yes/No ²
		PEAK WORKING VOLTAGE (U) V _{peak}	PEAK WORKING VOLTAGE (U) V d.c.		

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
Primary to secondary SELV (metal shield removed)	2 x MOOP	488	--	3.000 Vac	No
Primary to PE	1 x MOOP	488	--	1.740 Vac	No
Primary to metal shield (functional earth)	2 x MOOP	488	--	3.000 Vac	No
Supplementary information: ¹ Alternatively, per the Table (i.e., __dc), a d.c. test voltage equal to the peak value of the a.c. test voltage used. ² A) Immediately after humidity treatment of 5.7, ME EQUIPMENT de-energized, B) after required sterilization PROCEDURE, ME EQUIPMENT de-energized, C) after reaching steady state operating temperature as during heating test of 11.1.1, and D) after relevant tests of 11.6 (i.e., overflow, spillage, leakage, ingress of water, cleaning, disinfection, and sterilization).					
Supplementary information: EUT was evaluated for Means Of Operator Protection (MOOP). Safety capacitors (Y1 type) provided between primary and secondary (CY3, CY4), between primary and PE (CY1, CY2, CYCY7, CY8) and between secondary and PE (CY5, CY6): CY3= CY4= 470 pF CY1= CY2= CY5= CY6= 1000 pF CY7= CY8= 470 pF					

8.8.4.1	TABLE: Resistance to heat - Ball pressure test of thermoplastic parts		P
	Allowed impression diameter (mm)	≤ 2 mm	—
	Force (N)	20	—
Part/material		Test temperature (°C)	Impression diameter (mm)
Supplementary information: Approved material used. See list of critical components for details.			

8.8.4.1	RM RESULTS TABLE: Mechanical strength and resistance to heat		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
8.8.4.1	RM RESULTS TABLE: Mechanical strength and resistance to heat		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.5			
Supplementary information: The risk management requirements of the standard were not addressed. Power supply unit is intended for building-in. shall be evaluated during end medical product approval.			

8.9.2	TABLE: Short circuiting of each single one of the CREEPAGE DISTANCES and AIR CLEARANCES for insulation in the MAINS PART between parts of opposite polarity in lieu of complying with the required measurements in 8.9.4			N/A
Specific areas of circuits short-circuited and test conditions		Test in lieu of CREEPAGE DISTANCE or AIR CLEARANCE ¹	HAZARDOUS SITUATION observed (i.e., fire hazard, shock hazard, explosion, discharge of parts, etc.)? Yes/No	Remarks
Supplementary information: Note 1: AC - AIR CLEARANCE CD - CREEPAGE DISTANCE				
Supplementary information: Creepage and clearance distances between parts of opposite polarity provided before mains fuses. After mains fuses, distances verified by short circuit. See Table 13.2 for details.				

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

8.9.3.2	Table: Thermal cycling tests on one sample of insulating compound forming solid insulation between conductive parts		N/A
Test Sequence No.	Each test duration and temperature	Dielectric test voltage (V = Test voltage in 8.8.3 times 1.6)	Dielectric strength test after humidity preconditioning per cl. 5.7 except for 48 h only, Breakdown: Yes/No
1	68 h at $T1 \pm 2\text{ °C} = \text{___}^{\circ}\text{C}^1$		
	1 h at $25\text{ °C} \pm 2\text{ °C}$		
	2 h at $0\text{ °C} \pm 2\text{ °C}$		
	1 or more h at $25\text{ °C} \pm 2\text{ °C}$		
2	68 h at $T1 \pm 2\text{ °C} = \text{___}^{\circ}\text{C}^1$		
	1 h at $25\text{ °C} \pm 2\text{ °C}$		
	2 h at $0\text{ °C} \pm 2\text{ °C}$		
	1 or more h at $25\text{ °C} \pm 2\text{ °C}$		
3	68 h at $T1 \pm 2\text{ °C} = \text{___}^{\circ}\text{C}^1$		
	1 h at $25\text{ °C} \pm 2\text{ °C}$		
	2 h at $0\text{ °C} \pm 2\text{ °C}$		
	1 or more h at $25\text{ °C} \pm 2\text{ °C}$		
4	68 h at $T1 \pm 2\text{ °C} = \text{___}^{\circ}\text{C}^1$		
	1 h at $25\text{ °C} \pm 2\text{ °C}$		
	2 h at $0\text{ °C} \pm 2\text{ °C}$		
	1 or more h at $25\text{ °C} \pm 2\text{ °C}$		

Supplementary information:

¹ T1 = 10 °C above the maximum temperature of relevant part determined per 11.1.1, or 85 °C, the higher of the two. 10 °C not added to T1 when temperature measured by an embedded thermocouple. Used gradual transition from one temperature to another.

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

8.9.3.4	Table: Thermal cycling tests on one sample of cemented joint (see 8.9.3.3)		N/A
Test Sequence No.	Each test duration and temperature	Dielectric test voltage (V = Test voltage in 8.8.3 times 1.6)	Dielectric strength test after humidity preconditioning per cl. 5.7 except for 48 h only, Breakdown: Yes/No
1	68 h at $T1 \pm 2\text{ }^{\circ}\text{C} = \text{ }^{\circ}\text{C}^1$		
	1 h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	2 h at $0\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	1 or more h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
2	68 h at $T1 \pm 2\text{ }^{\circ}\text{C} = \text{ }^{\circ}\text{C}^1$		
	1 h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	2 h at $0\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	1 or more h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
3	68 h at $T1 \pm 2\text{ }^{\circ}\text{C} = \text{ }^{\circ}\text{C}^1$		
	1 h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	2 h at $0\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	1 or more h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
4	68 h at $T1 \pm 2\text{ }^{\circ}\text{C} = \text{ }^{\circ}\text{C}^1$		
	1 h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	2 h at $0\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		
	1 or more h at $25\text{ }^{\circ}\text{C} \pm 2\text{ }^{\circ}\text{C}$		

Supplementary information:

¹ T1 = 10 °C above the maximum temperature of relevant part determined per 11.1.1, or 85 °C, the higher of the two. 10 °C not added to T1 when temperature measured by an embedded thermocouple. Used gradual transition from one temperature to another.

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

8.10	TABLE: List of critical components					P
Component/ Part No.	Manufacturer/ Trademark	Type No./model No./	Technical data	Standard No./, Edition	Mark(s) & Certificates of conformity ¹	
Fuse (F1, F2) (for 65 W output power)	+ Walter	2010	Time delay 2 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40018781 UL E56092	
	Conquer	MST	Time delay 2 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40017118 UL E82636	
	Cooper Bussmann	SS-5	Time delay 2 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40031800 UL E19180	
	Bel Fuse inc.	RST	Time delay 2 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40011144 UL E20624	
	Littelfuse	392	Time delay 2 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 126983 UL E67006	
	SUN Electric Company	5T	Time delay 2 A / 250 Vac Soldered to PCB 5 x 20 mm	IEC/EN 60127 (JDYX2)	VDE 40027241 UL E166522	
	SUN Electric Company	5H	Time delay 2 A / 250 Vac Soldered to PCB 5 x 20 mm	IEC/EN 60127 (JDYX2)	VDE 40028239 UL E166522	
	Walter Electronic Co., Ltd.	TSD	Time delay 2 A / 250 Vac Soldered to PCB 5 x 20 mm	IEC/EN 60127 (JDYX2)	VDE 40001370 UL E56092	

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
Fuse (F1, F2) (for 80 W output power)	+ Walter	2010	Time delay 3.15 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40018781 UL E56092
	Conquer	MST	Time delay 3.15 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40017118 UL E82636
	Cooper Bussmann	SS-5	Time delay 3.15 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40031800 UL E19180
	Bel Fuse inc.	RST	Time delay 3.15 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 40011144 UL E20624
	Littelfuse	392	Time delay 3.15 A / 250 Vac Soldered to PCB 8,5 x 4 mm	IEC/EN 60127 (JDYX2)	VDE 126983 UL E67006
	SUN Electric Company	5T	Time delay 3.15 A / 250 Vac Soldered to PCB 5 x 20 mm	IEC/EN 60127 (JDYX2)	VDE 40027241 UL E166522
	SUN Electric Company	5H	Time delay 3.15 A / 250 Vac Soldered to PCB 5 x 20 mm	IEC/EN 60127 (JDYX2)	VDE 40028239 UL E166522
	Walter Electronic Co., Ltd.	TSD	Time delay 3.15 A / 250 Vac Soldered to PCB 5 x 20 mm	IEC/EN 60127 (JDYX2)	VDE 40001370 UL E56092

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
Capacitor (CY7, CY8) (for models with protective earth)	+ TDK	CD	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 138526 UL E37861
	SUCCESS Electronics Co. Ltd.	SE	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40008996 UL E114280
	JYA-NAY Co., Ltd.	JN	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001831 UL E201384
	Haohua Electronic Co.	CT7	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40003902 UL E233106
	Welson	WD	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40016157 UL E104572
	CHYUN FUH Electronic Co., Ltd.	CD	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001223 UL E202835
	Murata Mfg. Co., Ltd.	KX	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40002831 UL E379921
	ZHI WEI Electronics Co., Ltd.	DJ	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40032789 UL E330260
	Shantou High-New Technology Developmnt Zone Songtian Enterprise Co., Ltd.	CD	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40025754 UL E208107
	Walsin Technology Corp.	AH	Min.250 Vac Max.470 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001804 UL E146544
Capacitor (CX1)	+ Pilkor Electronics Co., Ltd.	PCX2	Min. 250 Vac Max. 0,15 µF Min X2 or X1	IEC/EN 60384-14 (FOWX2)	SEMKO SE/0256-1 UL E165646

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
	Ultra Tech Xiphi Enterprise Co., Ltd.	HQX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40024534 UL E183780
	Ultra Tech Xiphi	UTX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40023119 UL E183780
	Dain Electronics Co., Ltd.	MPX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40018798 UL E147776
	Shantou High-New Technology Development Zone Songtian Enterprise Co., Ltd.	MPX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40034679 UL E208107
	Cheng Tung Industrial	CTX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40022642 UL E193049
	Tenta Electric Industrial Co. Ltd.	MEX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 119119 UL E222911
Varistor (VDR1)	+ Success Electronics	SVR7D471K	300 Vrms; 385 Vdc diameter: 7 mm	IEC/EN 61051-2 (VZCA2)	VDE 123677 UL E330256
	Success Electronics	SVR10D471K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 40030401 UL E330256
	Success Electronics	SVR10D511K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 40030401 UL E330256
	Success Electronics	SVR14D471K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 40030401 UL E330256
	Thinking	TVR07471	300 Vrms; 385 Vdc diameter: 7 mm	IEC/EN 61051-2 (VZCA2)	VDE 5944 UL E314979
	Thinking	TVR10471	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 5944 UL E314979

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
	Thinking	TVR10511	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 5944 UL E314979
	Thinking	TVR14471	300 Vrms; 385 Vdc diameter: 14 mm	IEC/EN 61051-2 (VZCA2)	VDE 5944 UL E314979
	Thinking	TVR14511	300 Vrms; 385 Vdc diameter: 14 mm	IEC/EN 61051-2 (VZCA2)	VDE 5944 UL E314979
	Centra	CNR-07D471K	300 Vrms; 385 Vdc diameter: 7 mm	IEC/EN 61051-2 (VZCA2)	VDE 40008220 UL E316325
	Centra	CNR-10D471K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 40008220 UL E316325
	Centra	CNR-10D511K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 40008220 UL E316325
	Centra	CNR-14D471K	300 Vrms; 385 Vdc diameter: 14 mm	IEC/EN 61051-2 (VZCA2)	VDE 40008220 UL E316325
	Joyin Co., Ltd.	JVR07N471K	300 Vrms; 385 Vdc diameter: 7 mm	IEC/EN 61051-2 (VZCA2)	VDE 5937 UL E325508
	Joyin Co., Ltd.	JVR10N471K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 5937 UL E325508
	Joyin Co., Ltd.	JVR10N511K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 5937 UL E325508
	Joyin Co., Ltd.	JVR14N471K	300 Vrms; 385 Vdc diameter: 14 mm	IEC/EN 61051-2 (VZCA2)	VDE 5937 UL E325508
	Ceramate Techn. Co., Ltd.	GNR07D471K	300 Vrms; 385 Vdc diameter: 7 mm	IEC/EN 61051-2 (VZCA2)	VDE 40031745 UL E315429
	Ceramate Techn. Co., Ltd.	GNR10D471K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 40031745 UL E315429

IEC 60601-1					
Clause	Requirement + Test			Result - Remark	Verdict
	Ceramate Techn. Co., Ltd.	GNR10D511K	300 Vrms; 385 Vdc diameter: 10 mm	IEC/EN 61051-2 (VZCA2)	VDE 40031745 UL E315429
	Ceramate Techn. Co., Ltd.	GNR14D471K	300 Vrms; 385 Vdc diameter: 14 mm	IEC/EN 61051-2 (VZCA2)	VDE 40031745 UL E315429
Resistor bleeding (R1, R2)	Various	Various	Max. 360 kΩ Min. 1/8 W	IEC/EN 60601-1	Accepted.
Inductor (LF1)	Open type construction. Globtek / Sunycore Electronics Company Ltd. / BOAM / ZhongTong / Hejia GTM2065-LF1 OD: 19,0 x 17,5 x 22,0 mm Min. 2 x 17 mH Class B (130°C)			IEC/EN 60601-1	Accepted.
-- Bobbin	+ Chang Chung Plastic Co., Ltd.	+ T375J	UL94-V0 at minimum 0,45 mm thickness RTI: 150°C	IEC/EN 60601-1 (QMFZ2)	Accepted. UL E59481
-- Insulation tape	+ Jingjiang Yahua Pressure Sensitive Glue Co., Ltd.	+ CT-280B	130°C	IEC/EN 60601-1 (OANZ2)	Accepted. UL E165111
Capacitor (CX2)	+ Pilkor Electronics Co., Ltd.	PCX2	Min. 250 Vac Max. 0,15 µF Min X2 or X1	IEC/EN 60384-14 (FOWX2)	SEMKO SE/0256-1 UL E165646
	Ultra Tech Xiphi Enterprise Co., Ltd.	HQX	Min. 250 Vac Max. 0,15 µF Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40024534 UL E183780
	Ultra Tech Xiphi	UTX	Min. 250 Vac Max. 0,15 µF Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40023119 UL E183780
	Dain Electronics Co., Ltd.	MPX	Min. 250 Vac Max. 0,15 µF Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40018798 UL E147776
	Shantou High-New Technology Development Zone Songtian Enterprise Co., Ltd.	MPX	Min. 250 Vac Max. 0,15 µF Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40034679 UL E208107

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
	Cheng Tung Industrial	CTX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 (FOWX2)	VDE 40022642 UL E193049
	Tenta Electric Industrial Co. Ltd.	MEX	Min. 250 Vac Max. 0,15 μ F Min X2 or X1	IEC/EN 60384-14 FOWX2)	VDE 119119 UL E222911
Resistor (RT1)	+ Nanjing Btvop Electronics Co., Ltd.	MF71	2,5 W \varnothing 8,0 mm 5 Ω at 25°C	IEC/EN 60601-1	Accepted.
	+ NTC	SCK	2,5 W \varnothing 8,0 mm 5 Ω at 25°C	IEC/EN 60601-1	Accepted.
Capacitor (CY1, CY2) (for models with protective earth)	+ TDK	CD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 138526 UL E37861
	SUCCESS Electronics Co. Ltd.	SE	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40008996 UL E114280
	JYA-NAY Co., Ltd.	JN	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001831 UL E201384
	Haohua Electronic Co.	CT7	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40003902 UL E233106
	Welson	WD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40016157 UL E104572
	CHYUN FUH Electronic Co., Ltd.	CD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001223 UL E202835
	Murata Mfg. Co., Ltd.	KX	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40002831 UL E379921

IEC 60601-1					
Clause	Requirement + Test			Result - Remark	Verdict
	ZHI WEI Electronics Co., Ltd.	DJ	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40032789 UL E330260
	Shantou High-New Technology Developmnt Zone Songtian Enterprise Co., Ltd.	CD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40025754 UL E208107
	Walsin Technology Corp.	AH	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001804 UL E146544
Inductor (LF2)	Magnet wire wound on ferrite core Globtek / Sunycore Electronics Company Ltd. / BOAM / ZhongTong / Hejia GTM2065-LF2 OD (approximately): 13,0 x 7,0 x 7,0 mm (core) Min. 2 x 50 µH Class B (130°C)			IEC/EN 60601-1	Accepted.
-- Wire	+ Wuxi Huajia Electrical Wires Co., Ltd.	+ 2UEW	130°C 0,50 mm	IEC/EN 60601-1 (OBMW2)	Accepted. UL E226829
Inductor (L1)	Magnet wire wound on bobbin Globtek / Sunycore Electronics Company Ltd. / BOAM / ZhongTong / Hejia GTM2065-L1 OD: 26,0 x 20 x 2,0 mm Min. 12 mH Class B (130°C)			IEC/EN 60601-1	Accepted.
-- Bobbin	+ Chang Chun	T375J	Rated min. 94V-1 at min thickness 0,45 mm RTI 150°C	IEC/EN 60601-1 (QMFZ2)	Accepted. UL E59481
-- Wire	+ Wuxi Huajia Electrical Wires Co., Ltd.	2UEW	0,50 mm 130°C	IEC/EN 60601-1 (OBMW2)	Accepted. UL E226829

IEC 60601-1					
Clause	Requirement + Test			Result - Remark	Verdict
Inductor (L1) (alternate)	Magnet wire wound on ferrite core Globtek / Sunycore Electronics Company Ltd. / BOAM / ZhongTong / Hejia GTM2065-L1 OD: 26,0 x 20 x 2,0 mm Min. 12 mH Class B (130°C)			IEC/EN 60601-1	Accepted.
-- Wire	+ Dong Yang Electronics Ind Co., Ltd.	+ 2UEW	130°C 0,65 mm	IEC/EN 60601-1 (OBMW2)	Accepted. UL E102761
	Shanghai Asia Pacific Electric Co., Ltd.	2UEW	130°C 0,65 mm	IEC/EN 60601-1 (OBMW2)	Accepted. UL E214423
-- Tube	+ Shenzhen Woer Heat- Shrinkable Material Co., Ltd.	--	Ø 21 mm 125°C	IEC/EN 60601-1 (YDPU2)	Accepted. UL E203950
Diode bridge (BD1)	DIOTEC Electronics Corp.	SBU 6J	Min. 600 V Min. 6 A Min. 150°C	IEC/EN 60601-1 (QQQX2)	Accepted. UL E124962
	Various	Various	Min. 600 V Min. 4 A Min. 130°C	IEC/EN 60601-1 (QQQX2)	Accepted. UL approved.
Capacitor (C1)	Samxon	KM series	Max. 150 µF Min. 400 V Min. 105°C 18,0 x 35,0 mm	IEC/EN 60601-1	Accepted.
	Various	Various	Max. 150 µF Min. 400 V Min. 105°C 18,0 x 35,0 mm	IEC/EN 60601-1	Accepted.
Transistor (Q1)	Various	Various	Min. 10 A Min. 600 V	IEC/EN 60601-1	Accepted.
Optocoupler (U2, U4)	+ Lite-On	LTV-817	Clearance/creepage distance: 7,0 mm min. 5000 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 94722 UL E113898

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
	Fairchild	H11A817B	Clearance/creepage distance: 7,0 mm min. 5000 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 104801 UL E90700
	Fairchild	FOD817C	Clearance/creepage distance: 7,0 mm min. 5000 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 40026857 UL E90700
	Everlight Electronics Co., Ltd.	EL817	Clearance/creepage distance: 7,6 mm min. 5000 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 132249 UL E214129
	Cosmo Electronics Corp.	K1010	Clearance/creepage distance: 6,5 mm min. 5300 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 101347 UL E169586
	Cosmo Electronics Corp.	KP1010	Clearance/creepage distance: 6,5 mm min. 5300 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 101347 UL E169586
	Sharp	PC817	Clearance/creepage distance: 6,4 mm min. 5000 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 40008087 UL E64380
	Bright LED Electronics Corp.	BPC-817	Clearance/creepage distance: 7,6 mm min. 5000 Vac 100°C	IEC/EN 60747 (FPQU2)	VDE 40007240 UL E64380
Capacitor (CY3, CY4)	+ TDK	CD	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 138526 UL E37861
	SUCCESS Electronics Co. Ltd.	SE	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40008996 UL E114280

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
	JYA-NAY Co., Ltd.	JN	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40001831 UL E201384
	Haohua Electronic Co.	CT7	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40003902 UL E233106
	Welson	WD	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40016157 UL E104572
	CHYUN FUH Electronic Co., Ltd.	CD	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40001223 UL E202835
	Murata Mfg. Co., Ltd.	KX	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40002831 UL E379921
	ZHI WEI Electronics Co., Ltd.	DJ	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40032789 UL E330260
	Shantou High-New Technology Developmnt Zone Songtian Enterprise Co., Ltd.	CD	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40025754 UL E208107
	Walsin Technology Corp.	AH	Min.250 Vac Max.470 pF Min. Y1	IEC/EN 60384-14 (FOWX2)	VDE 40001804 UL E146544

IEC 60601-1					
Clause	Requirement + Test			Result - Remark	Verdict
Transformer (T1)	Open type construction GT(M)2065403.3 GT(M)20654005 GT(M)2065657.5 GT(M)20656509 GT(M)20656512 GT(M)20656515 GT(M)20656518 GT(M)20656524 GT(M)20656536 GT(M)20656548 +GlobTek or BOAM or Hejia or ZhongTong Primary: enamelled copper wire Secondary: triple insulated wire: + Great Leoflon, TRW-B or + COSMOLINK CO., LTD., TIW-M or + FURUKAWA, TEX-E Bobbin: Phenolic, (QMFZ2) UR E59481, type +T373J, T375J from Chang Chun, rated min. 94V-1 at min thickness 0,45 mm, RTI 150°C or (QMFZ2) UR E41429, type PM-9820 from Sumitomo Bakelite, rated 94V-0 at min. 0,16 mm thickness, measured thickness: 0,5 mm; RTI=150°C or equivalent			IEC/EN 60601-1	Accepted.
Capacitor (C101, C102, C103, C104)	Samxon	KM series	Max. 470 µF Min. 35 V (for models with output voltage below 35 Vdc) Min. 50 V (for other models) Min. 105°C 10,0 x 20,0 mm	IEC/EN 60601-1	Accepted.
	Various	Various	Max. 470 µF Min. 35 V (for models with output voltage below 35 Vdc) Min. 50 V (for other models) Min. 105°C 10,0 x 20,0 mm	IEC/EN 60601-1	Accepted.

IEC 60601-1					
Clause	Requirement + Test			Result - Remark	Verdict
Inductor (L100)	Choke GTM2065-4*12 Globtek / Sunycore Electronics Company Ltd. / BOAM / ZhongTong / Hejia Min. 0,7 µH Class B (130°C)			IEC/EN 60601-1	Accepted.
-- Wire	+ Dong Yang Electronics Ind Co., Ltd.	+ 2UEW	130°C 0,8 mm	IEC/EN 60601-1 (OBMW2)	Accepted. UL E102761
	Shanghai Asia Pacific Electric Co., Ltd.	2UEW	130°C 0,8 mm	IEC/EN 60601-1 (OBMW2)	Accepted. UL E214423
Capacitor (CY5, CY6) (for models with protective earth)	+ TDK	CD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 138526 UL E37861
	SUCCESS Electronics Co. Ltd.	SE	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40008996 UL E114280
	JYA-NAY Co., Ltd.	JN	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001831 UL E201384
	Haohua Electronic Co.	CT7	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40003902 UL E233106
	Welson	WD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40016157 UL E104572
	CHYUN FUH Electronic Co., Ltd.	CD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001223 UL E202835
	Murata Mfg. Co., Ltd.	KX	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40002831 UL E379921
	ZHI WEI Electronics Co., Ltd.	DJ	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40032789 UL E330260

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
	Shantou High-New Technology Developmnt Zone Songtian Enterprise Co., Ltd.	CD	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40025754 UL E208107
	Walsin Technology Corp.	AH	Min.250 Vac Max.1000 pF Min. Y2	IEC/EN 60384-14 (FOWX2)	VDE 40001804 UL E146544
Input connector (CON1)	+ Molex Electronics	A-41791 series 26-60-4030	UL94-V0 7 A / 250 Vac per contact 2 pins	IEC/EN 60601-1 (ECBT2)	Accepted. UL E29179
Output connector (CON3)	+ Molex Electronics	A-42227 series 26-60-4060	UL94-V0 4 A / 250 Vac per contact 6 pins	IEC/EN 60601-1 (ECBT2)	Accepted. UL E29179
	Joint Tech Electronic	A2542 series	UL94-V0 4 A / 250 Vac per contact 6 pins	IEC/EN 60601-1 (ECBT2)	Accepted. UL E179987
Printed circuit board (PCB)	Yuanman Printed Circuit Co., Ltd.	1V0	Min. UL94-V0 Min. 130°C 127,0 x 76,0 mm Min. thickness: 1,6 mm	(ZPMV2)	UL E74757
	Various	Various	Min. UL94-V0 Min. 130°C 127,0 x 76,0 mm Min. thickness: 1,6 mm	(ZPMV2)	UL approved
EMC shield (for models with protective earth)	Cheerful	02	Min. UL94-V0 Min. 130°C Copper provided on outer side. 127,0 x 76,0 mm Min. thickness: 1,0 mm Distance between edge and cooper: 4,8 mm	(ZPMV2)	UL E19724

IEC 60601-1					
Clause	Requirement + Test			Result - Remark	Verdict
	Various	Various	Min. UL94-V0 Min. 130°C Copper provided on outer side. 127,0 x 76,0 mm Min. thickness: 1,0 mm Distance between edge and cooper: 4,8 mm	(ZPMV2)	UL approved
PE conductor (for models with protective earth)	Various	Various	Min. 18 AWG Min. 80°C Green/yellow insulation	IEC/EN 60601-1 (AVLV2)	Accepted UL approved
Heatsink (for D101)	Aluminium GTM2065-HS1 OD: 50,0 x 19,0 x 24 mm			IEC/EN 60601-1	Accepted.
Heatsink (for Q1)	Aluminium GTM2065-HS1 OD: 50,0 x 19,0 x 24 mm			IEC/EN 60601-1	Accepted.
Supplementary information: 1) An asterisk indicates a mark which assures the agreed level of surveillance. See Licenses and Certificates of Conformity for verification.					

8.10.1	RM RESULTS TABLE: Fixing of components		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: All internal components mounted securely. Some components are additionally fixed with glue to prevent bending and therefore reduction of creepage / clearance distances.			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

8.10.2	RM RESULTS TABLE: Fixing of wiring		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			

Supplementary information:

Only PE conductor provided (connected between JZA and JZB).

Through the hole method used in addition to soldering. See enclosed pictures of the unit for details.

8.10.5	RM RESULTS TABLE: Mechanical protection of wiring		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			

Supplementary information:

No moving parts provided.

8.11.3.5	TABLE: Cord anchorages				N/A
Cord under test	Mass of equipment (kg)	Pull (N)	Torque Nm)	Remarks	

Supplementary information:

No cord anchorage provided. Power supply unit is intended for building-in.

8.11.3.6	TABLE: Cord guard				N/A
Cord under test	Test mass	Measured curvature	Remarks		

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Supplementary information:			
Power supply unit is intended for building-in.			

8.11.5	RM RESULTS TABLE: Mains fuses and over-current releases		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
Power supply unit is Class I equipment.			
Primary fuse is both supply leads provided inside the equipment. Refer to list of critical components for details.			

9.2.1	RM RESULTS TABLE: HAZARDS associated with moving parts – General		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
No moving parts.			

9.2.2.2	TABLE: Measurement of gap “a” according to Table 20 (ISO 13852: 1996)				N/A
Part of body	Allowable adult gap ¹ , mm	Measured adult gap, mm	Allowable children gap ¹ , mm	Measured children gap, mm	

IEC 60601-1				
Clause	Requirement + Test		Result - Remark	Verdict
Body	> 500		> 500	
Head	> 300 or < 120		> 300 or < 60	
Leg	> 180		> 180	
Foot	> 120 or < 35		> 120 or < 25	
Toes	> 50		> 50	
Arm	> 120		> 120	
Hand, wrist, fist	> 100		> 100	
Finger	> 25 or < 8		> 25 or < 4	
Supplementary information: ¹ In general, gaps for adults used, except when the device is specifically designed for use with children, values for children applied.				

9.2.2.4.3	RM RESULTS TABLE: Movable guards		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: No movable guards provided.			

9.2.2.4.4	RM RESULTS TABLE: Protective measures		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

9.2.2.5 c)	RM RESULTS TABLE: Continuous activation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.2.2.6	RM RESULTS TABLE: Speed of movement(s)		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.2.3.2	RM RESULTS TABLE: Over travel		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.2.3.2	RM RESULTS TABLE: Over travel		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
6.5			
Supplementary information: /			

9.2.4	RM RESULTS TABLE: Emergency stopping devices		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
6.6			
Supplementary information:			
No emergency stopping devices provided. EUT is power supply unit intended for building-in.			

9.2.5	RM RESULTS TABLE: Release of patient		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.3	RM RESULTS TABLE: Hazards associated with surfaces, corners and edges		P
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict

IEC 60601-1			
Clause	Requirement + Test		Verdict
9.3	RM RESULTS TABLE: Hazards associated with surfaces, corners and edges		P
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
No rough surfaces, no sharp corners and no sharp edges.			

9.4.2.1	TABLE: Instability—overbalance in transport position		N/A
ME EQUIPMENT preparation	Test Condition (transport position)	Remarks	
Supplementary information: /			

9.4.2.2	TABLE: Instability—overbalance excluding transport position		N/A
ME EQUIPMENT preparation	Test Condition (excluding transport position) Test either 5 ° incline and verify Warning marking or 10 ° incline)	Remarks	
Supplementary information: /			

9.4.2.3	TABLE: Instability—overbalance from horizontal and vertical forces		N/A
ME EQUIPMENT preparation	Test Condition (force used, direction of force, weight of equipment, location of force	Remarks	
Supplementary information: /			

9.4.2.4.2	TABLE: Castors and wheels – Force for propulsion		N/A
ME EQUIPMENT preparation	Test Condition (force location and height)	Remarks	
Supplementary information: /			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.4.2.4.3	TABLE: Castors and wheels – Movement over a threshold		N/A
ME EQUIPMENT preparation		Test Condition (speed of movement)	Remarks
Supplementary information: /			

9.4.2.4.3	RM RESULTS TABLE: Movement over a threshold		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.4.3.1	TABLE: Instability from unwanted lateral movement (including sliding) in transport position		N/A
ME EQUIPMENT Preparation	Test Condition (transport position, working load, locking device(s), caster position)	Remarks	
Supplementary information: /			

9.4.3.2	TABLE: Instability from unwanted lateral movement (including sliding) excluding transport position		N/A
ME EQUIPMENT Preparation	Test Condition (working load, locking device(s), caster position, force, force location, force direction)	Remarks	
Supplementary information: /			

9.4.4	TABLE: Grips and other handling devices		N/A
Clause and Name of Test	Test Condition	Remarks	

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

Supplementary information:

No grips and other handling devices provided.

9.5.1	RM RESULTS TABLE: Protective means		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.6.1	RM RESULTS TABLE: Acoustic energy – General		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.6.2.2	RM RESULTS TABLE: Infrasound and ultrasound energy		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.6.2.2	RM RESULTS TABLE: Infrasound and ultrasound energy		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
6.4			
6.5			
Supplementary information: /			

9.7.2	RM RESULTS TABLE: Pneumatic and hydraulic parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.7.4	RM RESULTS TABLE: Pressure rating of ME equipment parts		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.7.5	TABLE: Pressure vessels					N/A
Hydraulic, Pneumatic or Suitable Media and Test Pressure	Vessel Burst	Permanent Deformation	Leaks	Vessel fluid substance	Remarks	

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.7.5	TABLE: Pressure vessels		N/A
Supplementary Information: No pressure vessels provided.			

9.7.6	RM RESULTS TABLE: Pressure-control device		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: No such control devices provided.			

9.7.7	RM RESULTS TABLE: Pressure-relief device		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.8.1	RM RESULTS TABLE: Hazards associated with support systems - General		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.8.1	RM RESULTS TABLE: Hazards associated with support systems - General		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
6.3			
6.4			
6.5			
Supplementary information: /			

9.8.2	RM RESULTS TABLE: Tensile safety factor		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.8.3.1	RM RESULTS TABLE: Strength of patient or operator support or suspension systems – General		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.8.3.2	TABLE: PATIENT support/suspension system - Static forces				N/A
ME EQUIPMENT part or area	Position	Load	Area	Remarks	

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.8.3.2	TABLE: PATIENT support/suspension system - Static forces		N/A
Supplementary Information: /			

9.8.3.2a, b	RM RESULTS TABLE: Static forces due to loading from persons		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.8.3.3	TABLE: Support/Suspension System – Dynamic forces due to loading from persons			N/A
ME EQUIPMENT part or area	Position	Safe Working Load	Area	Remarks
Supplementary Information: /				

9.8.4.1	RM RESULTS TABLE: Systems with mechanical protective devices - General		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.8.4.3	RM RESULTS TABLE: Mechanical protective device for single activation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
9.8.4.3	RM RESULTS TABLE: Mechanical protective device for single activation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

9.8.5	RM RESULTS TABLE: Systems without mechanical protective devices		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

10.1.1	TABLE: Measurement of X – radiation		N/A
Maximum allowable radiation pA/kg (μSv/h) (mR/h)		36 (5 μSv/h) (0.5 mR/h)	
Surface area under test Surface no./ Description ¹		Measured Radiation, pA/kg (μSv/h) (mR/h)	Remarks
1/ /			
2/ /			
3/ /			
4/ /			
5/ /			
6/ /			
7/ /			
8/ /			
9/ /			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
10/ /			
Supplementary information: ¹ Measurements made at a distance of 5 cm from any surface to which OPERATOR (other than SERVICE PERSONNEL) can gain access without a TOOL, is deliberately provided with means of access, or is instructed to enter regardless of whether or not a TOOL is needed to gain access			

10.1.2	RM RESULTS TABLE: ME equipment intended to produce diagnostic or therapeutic X-radiation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

10.2	RM RESULTS TABLE: Alpha, beta, gamma, neutron & other particle radiation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: EUT not produces radiation. EUT is medical power supply unit intended for building-in.			

10.3	RM RESULTS TABLE: Microwave radiation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
10.3	RM RESULTS TABLE: Microwave radiation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

10.5	RM RESULTS TABLE: Other visible electromagnetic radiation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

10.6	RM RESULTS TABLE: Risk associated with infrared radiation other than emitted by lasers and LEDs		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

IEC 60601-1			
Clause	Requirement + Test		Verdict
10.7	RM RESULTS TABLE: RISK associated with ultraviolet radiation other than emitted by lasers and LEDs		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result – Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~) :	90	100	90	100	—
	Frequency (Hz) :	50	50	50	50	—
	Ambient T (°C) :	43,9	43,6	45	45	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-333.3-F						
1) Inductor L1		56,0	55,0	57,1	56,4	105
2) PCB near to diode bridge BD1		78,5	75,6	79,6	77,0	130
3) PCB near to diode D1		99,9	98,4	101,0	99,8	130
4) inductor LF1		80,3	76,8	81,4	78,2	105
5) Capacitor CX2		74,5	72,6	75,6	74,0	100
6) Transistor Q1		83,9	82,5	85,0	83,9	--
7) Bulk capacitor C1		73,3	72,4	74,4	73,8	105
8) Transformer T1 core		96,7	95,4	97,8	96,8	--
9) Transformer T1 windings		99,3	97,5	100,4	98,9	120
10) Optocoupler U2		79,6	78,7	80,7	80,1	100
11) Capacitor CY4		88,3	86,9	89,4	88,3	125
12) Output capacitor C101		98,4	96,3	99,5	97,7	105
13) PCB near to transistor Q1		84,0	82,5	85,1	83,9	130
14) Output diode D101		114,2	112,8	115,3	114,2	--
15) PCB near to output diode D101		107,4	105,9	108,5	107,3	130
Input current (A)		1,01	0,94	1,01	0,94	--
Output load		9,7 A / 3,3 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 45°C (without air flow).						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~):	90	264	90	264	—
	Frequency (Hz):	60	60	60	60	—
	Ambient T (°C):	43,7	43,7	45	45	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-333.3-F						
1) Inductor L1		56,3	51,5	57,6	52,8	105
2) PCB near to diode bridge BD1		78,0	65,0	79,3	66,3	130
3) PCB near to diode D1		99,8	105,5	101,1	106,8	130
4) inductor LF1		81,5	62,0	82,8	63,3	105
5) Capacitor CX2		75,0	61,9	76,3	63,2	100
6) Transistor Q1		83,8	91,2	85,1	92,5	--
7) Bulk capacitor C1		73,3	70,6	74,6	71,9	105
8) Transformer T1 core		96,8	96,6	98,1	97,9	--
9) Transformer T1 windings		98,8	98,2	100,1	99,5	120
10) Optocoupler U2		79,4	80,1	80,7	81,4	100
11) Capacitor CY4		88,3	87,2	89,6	88,5	125
12) Output capacitor C101		98,1	91,9	99,4	93,2	105
13) PCB near to transistor Q1		83,8	87,3	85,1	88,6	130
14) Output diode D101		114,1	109,6	115,4	110,9	--
15) PCB near to output diode D101		107,3	103,0	108,6	104,3	130
Input current (A)		1,03	0,43	1,03	0,43	--
Output load		9,7 A / 3,3 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 45°C (without air flow).						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~) :	240	264	240	264	—
	Frequency (Hz) :	50	50	50	50	—
	Ambient T (°C) :	43,9	43,7	45	45	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-333.3-F						
1) Inductor L1		51,6	51,2	52,7	52,5	105
2) PCB near to diode bridge BD1		65,6	64,8	66,7	66,1	130
3) PCB near to diode D1		103,4	105,1	104,5	106,4	130
4) inductor LF1		62,3	61,6	63,4	62,9	105
5) Capacitor CX2		62,5	61,8	63,6	63,1	100
6) Transistor Q1		88,9	90,4	90,0	91,7	--
7) Bulk capacitor C1		70,5	69,9	71,6	71,2	105
8) Transformer T1 core		96,1	95,6	97,2	96,9	--
9) Transformer T1 windings		98,2	97,1	99,3	98,4	120
10) Optocoupler U2		79,7	79,4	80,8	80,7	100
11) Capacitor CY4		86,6	86,2	87,7	87,5	125
12) Output capacitor C101		92,3	91,1	93,4	92,4	105
13) PCB near to transistor Q1		85,8	86,8	86,9	88,1	130
14) Output diode D101		110,2	108,9	111,3	110,2	--
15) PCB near to output diode D101		103,5	102,2	104,6	103,5	130
Input current (A)		0,47	0,43	0,47	0,43	--
Output load		9,7 A / 3,3 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 45°C (without air flow).						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~):	90	100	90	100	—
	Frequency (Hz):	50	50	50	50	—
	Ambient T (°C):	43,9	43,6	45	45	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-6548-F						
1) Inductor L1		63,5	61,5	64,6	62,9	105
2) PCB near to diode bridge BD1		93,0	88,1	94,1	89,5	130
3) PCB near to diode D1		100,3	96,1	101,4	97,5	130
4) inductor LF1		100,2	92,6	101,3	94,0	105
5) Capacitor CX2		86,5	82,7	87,6	84,1	100
6) Transistor Q1		89,2	86,0	90,3	87,4	--
7) Bulk capacitor C1		67,9	66,8	69,0	68,2	105
8) Transformer T1 core		88,3	86,4	89,4	87,8	--
9) Transformer T1 windings		95,6	93,1	96,7	94,5	120
10) Optocoupler U2		73,7	72,9	74,8	74,3	100
11) Capacitor CY4		79,9	78,2	81,0	79,6	125
12) Output capacitor C101		71,7	71,0	72,8	72,4	105
13) PCB near to transistor Q1		88,5	85,1	89,6	86,5	130
14) Output diode D101		94,5	94,2	95,6	95,6	--
15) PCB near to output diode D101		99,1	99,1	100,2	100,5	130
Input current (A)		1,42	1,31	1,42	1,31	--
Output load		1,36 A / 48,0 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 45°C (without air flow).						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~) :	90	264	90	264	—
	Frequency (Hz) :	60	60	60	60	—
	Ambient T (°C) :	43,7	43,7	45	45	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-6548-F						
1) Inductor L1		63,3	55,7	64,6	57,0	105
2) PCB near to diode bridge BD1		91,9	70,0	93,2	71,3	130
3) PCB near to diode D1		98,4	104,1	99,7	105,4	130
4) inductor LF1		100,6	65,2	101,9	66,5	105
5) Capacitor CX2		86,8	65,2	88,1	66,5	100
6) Transistor Q1		87,8	102,6	89,1	103,9	--
7) Bulk capacitor C1		67,4	68,8	68,7	70,1	105
8) Transformer T1 core		87,4	99,6	88,7	100,9	--
9) Transformer T1 windings		94,4	106,8	95,7	108,1	120
10) Optocoupler U2		73,5	80,0	74,8	81,3	100
11) Capacitor CY4		79,3	87,1	80,6	88,4	125
12) Output capacitor C101		71,8	76,9	73,1	78,2	105
13) PCB near to transistor Q1		87,3	95,5	88,6	96,8	130
14) Output diode D101		94,2	111,0	95,5	112,3	--
15) PCB near to output diode D101		98,8	128,4	100,1	129,7 *)	130
Input current (A)		1,44	0,64	1,44	0,64	--
Output load		1,36 A / 48,0 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
*) It is not possible to state compliance using a 95% coverage probability for the expanded uncertainty. Expanded uncertainty: U = 3°C (coverage factor kp = 2; confidence level: 95 %).						
Maximum ambient temperature specified by the manufacturer: 45°C (without air flow).						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~):	240	264	240	264	—
	Frequency (Hz):	50	50	50	50	—
	Ambient T (°C):	43,9	43,7	45	45	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-6548-F						
1) Inductor L1		55,6	55,3	56,7	56,6	105
2) PCB near to diode bridge BD1		70,7	70,1	71,8	71,4	130
3) PCB near to diode D1		100,5	103,4	101,6	104,7	130
4) inductor LF1		66,3	65,1	67,4	66,4	105
5) Capacitor CX2		65,1	64,5	66,2	65,8	100
6) Transistor Q1		97,2	101,9	98,3	103,2	--
7) Bulk capacitor C1		67,7	68,5	68,8	69,8	105
8) Transformer T1 core		96,9	99,0	98,0	100,3	--
9) Transformer T1 windings		103,5	105,8	104,6	107,1	120
10) Optocoupler U2		78,2	78,9	79,3	80,2	100
11) Capacitor CY4		84,5	86,3	85,6	87,6	125
12) Output capacitor C101		75,6	76,5	76,7	77,8	105
13) PCB near to transistor Q1		91,8	94,7	92,9	96,0	130
14) Output diode D101		108,4	110,4	109,5	111,7	--
15) PCB near to output diode D101		124,7	127,2	125,8 *)	128,5 *)	130
Input current (A)		0,69	0,64	0,69	0,64	--
Output load		9,7 A / 3,3 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
*) It is not possible to state compliance using a 95% coverage probability for the expanded uncertainty. Expanded uncertainty: U = 3°C (coverage factor kp = 2; confidence level: 95 %).						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~) :	90 **)	100 *)	90	100	—
	Frequency (Hz) :	50	50	50	50	—
	Ambient T (°C) :	48,7	48,7	50	50	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-553.3-FA						
1) Inductor L1		60,4	60,0	61,7	61,3	105
2) PCB near to diode bridge BD1		76,1	75,0	77,4	76,3	130
3) PCB near to diode D1		80,1	80,4	81,4	81,7	130
4) inductor LF1		72,0	70,9	73,3	72,2	105
5) Capacitor CX2		66,6	65,9	67,9	67,2	100
6) Transistor Q1		63,4	63,4	64,7	64,7	--
7) Bulk capacitor C1		66,2	66,1	67,5	67,4	105
8) Transformer T1 core		67,0	67,3	68,3	68,6	--
9) Transformer T1 windings		81,7	81,9	83,0	83,2	120
10) Optocoupler U2		50,6	50,7	51,9	52,0	100
11) Capacitor CY4		71,1	71,3	72,4	72,6	125
12) Output capacitor C101		93,7	93,6	95,0	94,9	105
13) PCB near to transistor Q1		63,6	63,5	64,9	64,8	130
14) Output diode D101		80,1	80,5	81,4	81,8	--
15) PCB near to output diode D101		79,8	80,1	81,1	81,4	130
Input current (A)		1,38	1,35	1,38	1,35	--
Output load		16,67 A / 3,3 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 50°C (with 10 CFM air flow).						
Unit was cooled with fan (airflow 10 CFM), placed on the transformer (T1) side of the supply, so the direction of the airflow was towards the transformer T1.						
*) Output decreased to 16,0 A.						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

****)** Output decreased to 15,7 A.

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~) :	90 **)	264			—
	Frequency (Hz) :	60	60			—
	Ambient T (°C) :	48,7	48,5			—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-553.3-FA						
1) Inductor L1		60,8	54,5	62,1	56	105
2) PCB near to diode bridge BD1		76,3	62,6	77,6	64,1	130
3) PCB near to diode D1		80,4	81,3	81,7	82,8	130
4) inductor LF1		73,7	55,0	75,0	56,5	105
5) Capacitor CX2		67,3	56,1	68,6	57,6	100
6) Transistor Q1		63,4	65,9	64,7	67,4	--
7) Bulk capacitor C1		66,1	62,0	67,4	63,5	105
8) Transformer T1 core		67,0	66,5	68,3	68,0	--
9) Transformer T1 windings		81,7	78,7	83,0	80,2	120
10) Optocoupler U2		50,6	50,8	51,9	52,3	100
11) Capacitor CY4		71,0	68,8	72,3	70,3	125
12) Output capacitor C101		93,7	84,9	95,0	86,4	105
13) PCB near to transistor Q1		63,6	63,6	64,9	65,1	130
14) Output diode D101		80,2	78,7	81,5	80,2	--
15) PCB near to output diode D101		79,9	77,1	81,2	78,6	130
Input current (A)		1,43	0,64	1,43	0,64	--
Output load		16,67 A / 3,3 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 50°C (with 10 CFM air flow).						
Unit was cooled with fan (airflow 10 CFM), placed on the transformer (T1) side of the supply, so the direction of the airflow was towards the transformer T1.						
**) Output decreased to 15,7 A.						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~):	240	264	240	264	—
	Frequency (Hz):	50	50	50	50	—
	Ambient T (°C):	48,6	48,5	50	50	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-553.3-FA						
1) Inductor L1		54,8	54,3	56,2	55,8	105
2) PCB near to diode bridge BD1		63,1	62,4	64,5	63,9	130
3) PCB near to diode D1		80,5	81,4	81,9	82,9	130
4) inductor LF1		55,9	55,1	57,3	56,6	105
5) Capacitor CX2		56,9	56,2	58,3	57,7	100
6) Transistor Q1		64,9	65,9	66,3	67,4	--
7) Bulk capacitor C1		62,3	62,0	63,7	63,5	105
8) Transformer T1 core		66,4	66,5	67,8	68,0	--
9) Transformer T1 windings		78,7	78,7	80,1	80,2	120
10) Optocoupler U2		50,9	50,8	52,3	52,3	100
11) Capacitor CY4		68,8	68,8	70,2	70,3	125
12) Output capacitor C101		85,8	85,1	87,2	86,6	105
13) PCB near to transistor Q1		63,0	63,7	64,4	65,2	130
14) Output diode D101		78,9	78,7	80,3	80,2	--
15) PCB near to output diode D101		77,5	77,2	78,9	78,7	130
Input current (A)		0,70	0,65	0,70	0,65	--
Output load		16,67 A / 3,3 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 50°C (with 10 CFM air flow).						
Unit was cooled with fan (airflow 10 CFM), placed on the transformer (T1) side of the supply, so the direction of the airflow was towards the transformer T1.						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~) :	90	100	90	100	—
	Frequency (Hz) :	50	50	50	50	—
	Ambient T (°C) :	48,7	48,7	50	50	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-8048-FA						
1) Inductor L1		62,3	60,6	63,6	61,9	105
2) PCB near to diode bridge BD1		85,5	81,4	86,8	82,7	130
3) PCB near to diode D1		70,6	68,2	71,9	69,5	130
4) inductor LF1		81,6	76,3	82,9	77,6	105
5) Capacitor CX2		77,9	74,0	79,2	75,3	100
6) Transistor Q1		65,8	64,0	67,1	65,3	--
7) Bulk capacitor C1		62,1	60,7	63,4	62,0	105
8) Transformer T1 core		70,4	68,1	71,7	69,4	--
9) Transformer T1 windings		75,0	71,9	76,3	73,2	120
10) Optocoupler U2		51,0	50,9	52,3	52,2	100
11) Capacitor CY4		61,3	60,2	62,6	61,5	125
12) Output capacitor C101		61,3	60,7	62,6	62,0	105
13) PCB near to transistor Q1		66,0	64,0	67,3	65,3	130
14) Output diode D101		75,7	75,7	77,0	77,0	--
15) PCB near to output diode D101		73,8	74,2	75,1	75,5	130
Input current (A)		1,67	1,53	1,67	1,53	--
Output load		1,67 A / 48 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 50°C (with 10 CFM air flow).						
Unit was cooled with fan (airflow 10 CFM), placed on the transformer (T1) side of the supply, so the direction of the airflow was towards the transformer T1.						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~):	90	264			—
	Frequency (Hz):	60	60			—
	Ambient T (°C):	48,7	48,5			—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-8048-FA						
1) Inductor L1		62,6	54,7	63,9	56,2	105
2) PCB near to diode bridge BD1		85,2	64,3	86,5	65,8	130
3) PCB near to diode D1		70,1	72,1	71,4	73,6	130
4) inductor LF1		82,9	56,1	84,2	57,6	105
5) Capacitor CX2		78,7	58,5	80,0	60,0	100
6) Transistor Q1		65,4	70,5	66,7	72,0	--
7) Bulk capacitor C1		61,6	57,8	62,9	59,3	105
8) Transformer T1 core		69,8	72,6	71,1	74,1	--
9) Transformer T1 windings		74,2	75,3	75,5	76,8	120
10) Optocoupler U2		51,0	51,4	52,3	52,9	100
11) Capacitor CY4		61,0	62,2	62,3	63,7	125
12) Output capacitor C101		61,1	62,8	62,4	64,3	105
13) PCB near to transistor Q1		65,6	66,0	66,9	67,5	130
14) Output diode D101		75,7	87,1	77,0	88,6	--
15) PCB near to output diode D101		73,7	97,1	75,0	98,6	130
Input current (A)		1,70	0,75	1,70	0,75	--
Output load		1,67 A / 48 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 50°C (with 10 CFM air flow).						
Unit was cooled with fan (airflow 10 CFM), placed on the transformer (T1) side of the supply, so the direction of the airflow was towards the transformer T1.						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	TABLE: Excessive temperatures in ME EQUIPMENT					P
	Supply voltage (V~) :	240	264	240	264	—
	Frequency (Hz) :	50	50	50	50	—
	Ambient T (°C) :	48,6	48,5	50	50	—
Maximum measured temperature T of part/at:		Max measured temperature (°C)		Max. measured temperature calculated to maximum ambient temperature (°C)		Allowed Tmax (°C)
Model: GTM2065-8048-FA						
1) Inductor L1		54,8	54,6	56,2	56,1	105
2) PCB near to diode bridge BD1		65,0	64,3	66,4	65,8	130
3) PCB near to diode D1		70,4	72,1	71,8	73,6	130
4) inductor LF1		57,1	56,2	58,5	57,7	105
5) Capacitor CX2		59,3	58,5	60,7	60,0	100
6) Transistor Q1		68,4	70,4	69,8	71,9	--
7) Bulk capacitor C1		57,7	57,9	59,1	59,4	105
8) Transformer T1 core		71,7	72,5	73,1	74,0	--
9) Transformer T1 windings		74,4	75,2	75,8	76,7	120
10) Optocoupler U2		51,4	51,4	52,8	52,9	100
11) Capacitor CY4		61,7	62,1	63,1	63,6	125
12) Output capacitor C101		62,4	62,7	63,8	64,2	105
13) PCB near to transistor Q1		64,8	65,9	66,2	67,4	130
14) Output diode D101		86,0	87,2	87,4	88,7	--
15) PCB near to output diode D101		94,4	96,9	95,8	98,4	130
Input current (A)		0,81	0,75	0,81	0,75	--
Output load		1,67 A / 48 Vdc				--
Supplementary information:						
Temperature rises of the transformer was measured with thermocouples (Class B transformer provided inside the unit, 130°C - 10°C= 120°C).						
The printed circuit board (PCB) is rated 130°C.						
Max temperature determined in accordance with 11.1.3e).						
Maximum ambient temperature specified by the manufacturer: 50°C (with 10 CFM air flow).						
Unit was cooled with fan (airflow 10 CFM), placed on the transformer (T1) side of the supply, so the direction of the airflow was towards the transformer T1.						

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

11.1.1	RM RESULTS TABLE: Maximum temperature during normal use (Table 23 or 24)		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
No external enclosure provided (power supply unit is intended for building-in).			

11.1.2.1	RM RESULTS TABLE: Applied parts intended to supply heat to patient		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
No applied parts. EUT is power supply unit intended for building-in.			

11.1.2.2	RM RESULTS TABLE: Applied parts not intended to supply heat to patient		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
11.1.2.2	RM RESULTS TABLE: Applied parts not intended to supply heat to patient		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
No applied parts. EUT is power supply unit intended for building-in.			

11.1.3	TABLE: Temperature of windings by change-of-resistance method						N/A
Temperature T of winding:	t ₁ (°C)	R ₁ (Ω)	t ₂ (°C)	R ₂ (Ω)	T (°C)	Allowed T _{max} (°C)	Insulation class
Primary windings	24,9	475,66 kΩ	24,4	509,70 kΩ	59,1 (Calculate to max. ambient 40°C)	105	Class A
Supplementary information:							
Switch mode transformer incorporated within the equipment. Temperature of transformer windings measured with thermocouplers.							

11.1.3	RM RESULTS TABLE: Measurements		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
Temperature measurements performed. Test corner not used because power supply unit is intended for building-in. Temperature tests were performed 100 mm above the bench.			

11.2.2.1	RM RESULTS TABLE: Risk of fire in an oxygen rich environment	N/A
----------	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
Not evaluated for use in an oxygen rich environment.			

11.2.2.1	TABLE: Alternative method to 11.2.2.1 a) 5) to determine existence of an ignition source		N/A
Areas where sparking might cause ignition:			Remarks
1.			
2.			
3.			
5.			
6.			
Materials of the parts between which sparks could occur (Composition, Grade Designation, Manufacturer):			Remarks
1.			
2.			
3.			
4.			
5.			
6.			
Test parameters selected representing worst case conditions for ME EQUIPMENT:			Remarks
Oxygen concentration (%)			
Fuel.....			
Current (A).....			
Voltage (V)			
Capacitance (μF).....			
Inductance or resistance (h or Ω)			
No. of trials (300 Min).....			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Sparks resulted in ignition (Yes/No) :			
Supplementary information: Test procedure of 11.2.2.1 a) 5) & Figs 35-37 used for tests. For circuits not in Figs 35-37, test voltage or current set at 3 times the worst case values with other parameters set at worst case values to determine if ignition can occur.			

11.3	RM RESULTS TABLE: Constructional requirements for fire enclosures of ME equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: Power supply unit is provided without external enclosure.			

11.5	RM RESULTS TABLE: ME equipment and ME systems intended for use in conjunction with flammable agents		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: The risk management requirements of the standard were not addressed. Power supply unit not evaluated for use in conjunction with flammable agents.			

11.6.1	TABLE: overflow, spillage, leakage, ingress of water, cleaning, disinfection, sterilization, compatibility with substances		N/A
--------	---	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

Clause / Test Name	Test Condition	Part under test	Remarks

Supplementary information:

EUT is intended for building-in provided without external enclosure. End product consideration.

11.6.2	RM RESULTS TABLE: Overflow in ME equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			

Supplementary information:

EUT is intended for building-in provided without external enclosure. End product consideration.

11.6.3	RM RESULTS TABLE: Spillage on ME equipment and ME system		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			

Supplementary information:

EUT is intended for building-in provided without external enclosure. End product consideration.

11.6.5	RM RESULTS TABLE: Ingress of water or particulate matter into ME EQUIPMENT and ME SYSTEMS		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
11.6.5	RM RESULTS TABLE: Ingress of water or particulate matter into ME EQUIPMENT and ME SYSTEMS		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
Supplementary information: EUT is intended for building-in provided without external enclosure. End product consideration.			

11.6.6	RM RESULTS TABLE: Cleaning and disinfection of ME equipment and ME systems		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: EUT is intended for building-in provided without external enclosure. End product consideration.			

11.6.7	RM RESULTS TABLE: Sterilization of ME equipment and ME systems		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: EUT is intended for building-in provided without external enclosure. End product consideration.			

11.6.8	RM RESULTS TABLE: Compatibility with substances used		N/E
--------	--	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: The risk management requirements of the standard were not addressed. EUT is intended for building-in provided without external enclosure. End product consideration.			

12.1	RM RESULTS TABLE: Accuracy of controls and equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: No controls provided. EUT is power supply unit intended for building-in.			

12.3	RM RESULTS TABLE: Alarm systems		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
12.3	RM RESULTS TABLE: Alarm systems		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.4			
6.5			
Supplementary information: No alarm incorporated.			

12.4.1	RM RESULTS TABLE: Intentional exceeding of safety limits		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

12.4.2	RM RESULTS TABLE: Indication of parameters relevant to safety		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: No energy delivered to the patient. No applied parts provided.			

12.4.3	RM RESULTS TABLE: Accidental selection of excessive output values		N/A
--------	---	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

12.4.4	RM RESULTS TABLE: Incorrect output		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information:			
EUT is power supply unit intended for building-in. During single fault conditions, output voltage was below SELV limit.			

12.4.5.2	RM RESULTS TABLE: Diagnostic X-ray equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
12.4.5.2	RM RESULTS TABLE: Diagnostic X-ray equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.5			
Supplementary information: EUT is not diagnostic X-ray equipment.			

12.4.5.3	RM RESULTS TABLE: Radiotherapy equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: EUT is not radiotherapy equipment.			

12.4.5.4	RM RESULTS TABLE: Other ME equipment producing diagnostic or therapeutic radiation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: EUT not produces diagnostic or therapeutic radiation.			

12.4.6	RM RESULTS TABLE: Diagnostic or therapeutic acoustic pressure		N/A
--------	---	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

13.1.2	TABLE: measurement of power or energy dissipation in parts & components to waive SINGLE FAULT CONDITIONS in 4.7, 8.1 b), 8.7.2, and 13.2.2 relative to emission of flames, molten metal, or ignitable substances			N/A
Power dissipated less than (W).....:		15		
Energy dissipated less than (J).....:		900		
Part or component tested	Measured power dissipated (W)	Calculated energy dissipated (J)	SINGLE FAULT CONDITIONS waived (Yes/No)	Remarks
Supplementary information: /				

13.2	TABLE: SINGLE FAULT CONDITIONS in accordance with 13.2.2 to 13.2.13, inclusive			P
Clause No.	Description of SINGLE FAULT CONDITION	Results observed	HAZARDOUS SITUATION (Yes/No)	
13.2.2	Electrical SINGLE FAULT CONDITIONS per Clause 8.1:	—	—	
	Diode D101 short (No load) Supply voltage: 264 Vac	Output switched off immediately. No hazard. Unit damaged.	No	
	Diode D101 short (Load) Supply voltage: 264 Vac	Output switched off immediately. No hazard. Unit damaged.	No	
	Inductor L100 short (No load) Supply voltage: 264 Vac	No effect on function.	No	

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Inductor L100 short (Load) Supply voltage: 264 Vac	No effect on function.	No
	Optocoupler U2 Pin 1 to Pin 2 short (No load) Supply voltage: 264 Vac	Unit went to hiccup mode. No defect. No hazard.	No
	Optocoupler U2 Pin 1 to Pin 2 short (Load) Supply voltage: 264 Vac	Output voltage increased to 51,7V and than decreased to 0V. No hazard. Unit damaged.	No
	Optocoupler U2 Pin 3 to Pin 4 short (No load) Supply voltage: 264 Vac	Output switched off immediately. No defect. No hazard.	No
	Optocoupler U2 Pin 3 to Pin 4 short (Load) Supply voltage: 264 Vac	Output switched off immediately. No defect. No hazard.	No
	Optocoupler U4 Pin 1 to Pin 2 short (No load) Supply voltage: 264 Vac	No effect on function.	No
	Optocoupler U4 Pin 1 to Pin 2 short (Load) Supply voltage: 264 Vac	No effect on function.	No
	Optocoupler U4 Pin 3 to Pin 4 short (No load) Supply voltage: 264 Vac	Output switched off immediately. No defect. No hazard.	No
	Optocoupler U4 Pin 3 to Pin 4 short (Load) Supply voltage: 264 Vac	Output switched off immediately. No defect. No hazard.	No
	Varistor VDR1 short Supply voltage: 264 Vac	Fuse F1, F2 opened immediately. No hazard.	No
	Capacitor CX2 short Supply voltage: 264 Vac	Fuse F1, F2 opened immediately. No hazard.	No
	Rectifier BD1 plus to minus short Supply voltage: 264 Vac	Fuse F1, F2 opened immediately. No hazard.	No

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Plus output to earth Supply voltage: 264 Vac	No effect on function.	No
	Minus output to earth Supply voltage: 264 Vac	No effect on function.	No
	Minus output to plus output Supply voltage: 264 Vac	Output switched off immediately. No defect, no hazard.	No
	Primary current sense R21 short Supply voltage: 264 Vac	Output switched off immediately. No hazard. Unit damaged.	No
	U1 Pin 7 to Pin 5 short Supply voltage: 264 Vac	Output switched off immediately. No defect. No hazard.	No
	Switching transistor Q1 D to S short Supply voltage: 264 Vac	Output switched off immediately. No hazard. Unit damaged.	No
	Switching transistor Q1 D to G short Supply voltage: 264 Vac	Output switched off immediately. No hazard. Unit damaged.	No
	Transformer T1 Pin 1,4 to Pin 2 short Supply voltage: 264 Vac	Unit went to hiccup mode. No defect. No hazard. No excessive temperature rise.	No
	Transformer T1 Pin 3 to Pin 6 short Supply voltage: 264 Vac	Output switched off immediately. No hazard. No excessive temperature rise. Unit damaged.	No
	Transformer T1 Pin 7,8 to Pin 10,11 short Supply voltage: 264 Vac	Output switched off immediately and tried to switch on. No hazard. No excessive temperature rise. Unit damaged.	No
	Transformer T1 Pin 7,8 to Pin 10,11 overload Supply voltage: 264 Vac	No secondary current limitation. Refer to output overload.	No

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
	Output overload Model: GTM2065-333.3-F Supply voltage: 264 Vac	Load on output: 19,0A @ 3,3Vdc. After 40min the output switched off. The measured temperature on T1 was 144,9°C at an ambient of 48,5°C. Calculated temperatures at maximum specified ambient is 146,4°C. Temperature limit: 175°C – 10°C = 165°C. 10°C were subtracted because of the measurement with the thermo probes. No defect. No hazard.	No
	Output overload Model: GTM2065-6548-F Supply voltage: 264 Vac	Load on output: 2,70A @ 44,9Vdc. After 60min the output decreased to 2,17A @ 36,23Vdc and remained. The measured temperature on T1 was 160,1°C at an ambient of 48,7°C. Calculated temperatures at maximum specified ambient is 161,4°C. Temperature limit: 175°C – 10°C = 165°C. 10°C were subtracted because of the measurement with the thermo probes. No defect. No hazard.	No
	Output short Model: GTM2065-333.3-F Supply voltage: 264 Vac	Output switched off immediately. No defect. No hazard.	No
	Output short Model: GTM2065-6548-F Supply voltage: 264 Vac	Output switched off immediately. No defect. No hazard.	No
13.2.3	Overheating of transformers per Clause 15.5:	—	—
	SEE TABLE 15.5.1.2 and 15.5.1.3 for details.		No

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
13.2.4	Failure of THERMOSTATS according to 13.2.13 & 15.4.2, overloading - THERMOSTATS short circuited or interrupted, the less favourable of the two:	—	—
13.2.5	Failure of temperature limiting devices according to 13.2.13 & 15.4.2, overloading, THERMOSTATS short circuited or interrupted, the less favourable of the two:	—	—
13.2.6	Leakage of liquid - RISK MANAGEMENT FILE examined to determine the appropriate test conditions (sealed rechargeable batteries exempted)	—	—
13.2.7	Impairment of cooling that could result in a HAZARD using test method of 11.1:	—	—
	Single ventilation fans locked consecutively		
	Ventilation openings on top and sides impaired by covering openings on top of ENCLOSURE or positioning of ME EQUIPMENT against walls		
	Simulated blocking of filters		
	Flow of a cooling agent interrupted		
13.2.8	Locking of moving parts – Only one part locked at a time – Also see 13.2.10 below:	—	—
13.2.9	Interruption and short circuiting of motor capacitors – Motor capacitors short & open circuited ¹ – Also see 13.10	—	—
13.2.10	Additional test criteria for motor operated ME EQUIPMENT in 13.2.8 & 13.2.9:	—	—
	For every test in SINGLE FAULT CONDITION of 13.2.8 and 13.2.9, motor-operated EQUIPMENT started from COLD CONDITION at RATED voltage or at the upper limit of RATED voltage range for specified time:		
	Temperatures of windings determined at the end of specified test periods or at the instant of operation of fuses, THERMAL CUT-OUTS, motor protective devices		
	Temperatures measured as specified in 11.1.3 d)		
	Temperatures did not exceed limits of Table 26		

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
13.2.11	Failures of components in ME EQUIPMENT used in conjunction with OXYGEN RICH ENVIRONMENTS:	—	—
13.2.12	Failure of parts that might result in a MECHANICAL HAZARD (See 9 & 15.3):	—	—
Supplementary information: ¹ Test with short-circuited capacitor not performed when motor provided with a capacitor complying with IEC 60252-1 and the ME EQUIPMENT not intended for unattended use including automatic or remote control. See Attachment # and appended Table 8.10. There was no flame, extensive smoke or melted metal. When components were failing, the test was repeated two times. *** Test was repeated 10 times Test time: The time until the effect occurred was recorded.			

13.2.6	RM RESULTS TABLE: Leakage of liquid		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

14.1	RM RESULTS TABLE: Programmable electrical medical systems - General		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary information: /			

14.6.1	RM RESULTS TABLE: Identification of known and foreseeable hazards	N/A
--------	---	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.3			
Supplementary information: /			

14.6.2	RM RESULTS TABLE: Risk control		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.1			
Supplementary information: /			

14.7	RM RESULTS TABLE: Requirement specification		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.3			
Supplementary information: /			

14.8	RM RESULTS TABLE: Architecture		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.3			
Supplementary information: /			

14.9	RM RESULTS TABLE: Design and Implementation		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.2			
6.3			
Supplementary information: /			

14.10	RM RESULTS TABLE: Verification		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.3			
Supplementary information: /			

14.11	RM RESULTS TABLE: PEMS validation		N/A
-------	-----------------------------------	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
6.3			
Supplementary information: /			

14.13	RM RESULTS TABLE: Connection of PEMS by NETWORK/DATA COUPLING to other equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
Supplementary information: /			

15.1	RM RESULTS TABLE: Construction of ME equipment – Arrangements of controls and indicators of ME equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

15.3	TABLE: Mechanical Strength tests ¹⁾			N/A
Clause	Name of Test	Test conditions	Observed results/Remarks	
Supplementary information: ¹⁾ As applicable, Push, Impact, Drop, Mould Stress Relief and Rough Handling Tests (delete not applicable rows).				
Power supply unit is provided without external enclosure. It is intended for building-in within end medical product.				

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.3.2	RM RESULTS TABLE: Push test		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary information: /			

15.3.3	RM RESULTS TABLE: Impact test		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary information: /			

15.3.4.2	RM RESULTS TABLE: Portable ME equipment		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary information: /			

15.3.5	RM RESULTS TABLE: Rough handling test		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary information: /			

15.4.1	RM RESULTS TABLE: Construction of connectors		N/A
--------	--	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: No such connectors provided.			

15.4.2.1 a	RM RESULTS TABLE: thermal cut-outs and over-current releases		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
Supplementary information: No such components incorporated within the power supply unit.			

15.4.2.1 b	RM RESULTS TABLE: THERMAL CUT-OUTS with a safety function		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary information: Non-resettable thermal cut-out incorporated within the power supply unit.			

15.4.2.1 c	RM RESULTS TABLE: Independent non-SELF-RESETTING THERMAL CUT-OUT		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			

IEC 60601-1			
Clause	Requirement + Test		Verdict
15.4.2.1 c	RM RESULTS TABLE: Independent non-SELF-RESETTING THERMAL CUT-OUT		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.4			
Supplementary information: No thermostats provided.			

15.4.2.1 d	RM RESULTS TABLE: Loss of function of ME EQUIPMENT		N/E
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary information: The risk management requirements of the standard were not addressed. End product consideration. Power supply unit is intended for building-in.			

15.4.2.1 h	RM RESULTS TABLE: ME EQUIPMENT with tubular heating elements		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary information: No such componnts incorporated within the power supplyl unit.			

15.4.3.1	RM RESULTS TABLE: Housing		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary information: /			

15.4.3.2	RM RESULTS TABLE: Connection		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.4.3.2	RM RESULTS TABLE: Connection		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.3			
4.4			
Supplementary information: /			

15.4.3.3	RM RESULTS TABLE: Protection against overcharging		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary information: /			

15.4.3.4	RM RESULTS TABLE: Lithium batteries		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
Supplementary information: /			

15.4.3.5	RM RESULTS TABLE: Excessive current and voltage protection		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

15.4.4	RM RESULTS TABLE: Indicators		N/E
--------	------------------------------	--	-----

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			

Supplementary information:

The risk management requirements of the standard were not addressed. EUT is not end medical product.

There is only green indicator light to indicate power on. Power supply unit is intended for building-in within end medical product.

15.4.5	RM RESULTS TABLE: Pre-set controls		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			

Supplementary information:

No pre-set controls provided.

15.4.6	TABLE: actuating parts of controls of ME EQUIPMENT – torque & axial pull tests					N/A
Rotating control under test	Gripping diameter “d” of control knob (mm) ¹	Torque from Table 30 (Nm)	Axial force applied (N)	Unacceptable RISK occurred Yes/No	Remarks	

Supplementary information: ¹ Gripping diameter (d) is the maximum width of a control knob regardless of its shape (e.g. control knob with pointer)

15.4.7.3 b	RM RESULTS TABLE: Entry of liquids		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
15.4.7.3 b	RM RESULTS TABLE: Entry of liquids		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.4			
Supplementary information: /			

15.5.1.2	TABLE: transformer short circuit test short-circuit applied at end of windings or at the first point that could be short circuited under SINGLE FAULT CONDITION						P
Primary voltage (most adverse value from 90 % to 110 % of RATED voltage)(V) ¹:						264	—
RATED input frequency (Hz).....:						50	—
Winding tested	Class of insulation (A, B, E, F, or H)	Type of protective device (fuse, circuit breaker) /Ratings	Protective device operated Yes/No	Time to THERMAL STABILITY (when protective device did not operate)(Min)	Maximum allowed temp from Table 31 (°C)	Maximum winding temp measured (°C)	Ambient (°C)
Transformer T1 (Pin 1,4 to Pin 2)	B	Input fuse	No	N/A	165	See *)	25
Transformer T1 (Pin 3 to Pin 6)	B	Input fuse	No	N/A	165	See **)	25
Transformer T1 (Pin 7,8 to Pin 10,11)	B	Input fuse	No	N/A	165	See ***)	25
Supplementary information: ¹ Loads on other windings between no load and their NORMAL USE load. Short-circuit applied at end of windings or at the first point that could be short circuited under SINGLE FAULT CONDITION.							
Supplementary information: *) Hic-cup mode of operation. No high temperature rises observed. No defect, no hazard. **) Output switched off immediately. No high temperature rises observed. No defect, no hazard. ***) Output switched off immediately and tried to switch on. No high temperature rises observed. Unit damaged. No hazard.							

15.5.1.3	TABLE: transformer overload test – conducted only when protective device under short-circuit test operated						P
Primary voltage, most adverse value between 90 % to 110 % of RATED voltage (V) ¹ ...:						264 Vac	
RATED input frequency (Hz).....:						50 Hz	
Test current just below minimum current that would activate protective device & achieve THERMAL STABILITY under method a) (A).....:						--	

IEC 60601-1					
Clause	Requirement + Test		Result - Remark		Verdict
Test current based on Table 32 when protective device that operated under method a) is external to transformer, and it was shunted (A)..... :					--
Winding tested	Class of insulation (A, B, E, F, H)	Type of protective device used (fuse, circuit breaker)/Ratings	Maximum allowed temp from Table 31 (°C)	Maximum winding temp measured (°C)	Ambient (°C)
Transformer T1 (Pin 7,8 to 10,11) Model: GTM2065-333.3-F	B	Input fuse	165	146,4	50
Transformer T1 (Pin 7,8 to 10,11) Model: GTM2065-6548-F	B	Input fuse	165	161,4	50
Supplementary information: ¹ Loads on other windings between no load and their NORMAL USE load. Time durations: - IEC 60127-1 fuse: 30 min at current from Table 32. Non IEC 60127-1 fuse: 30 min at the current based on characteristics supplied by fuse manufacturer, specifically, 30 min clearing-time current. When no 30 min clearing-time current data available, test current from Table 32 used until THERMAL STABILITY achieved. - Other types of protective devices: until THERMAL STABILITY achieved at a current just below minimum current operating the protective device in a). This portion concluded at specified time or when a second protective device opened.					
Supplementary information: No secondary current limitation; therefore output overload represents transformer overload. Class B transformer incorporated. Temperature limit: 175°C – 10°C = 165°C (10°C were subtracted because of the measurement with the thermo probes).					

15.5.2	TABLE: Transformer dielectric strength after humidity preconditioning of 5.7					N/A
Transformer Model/Type/ Part No	Test voltage applied between	Test voltage, (V)	Test frequency (Hz)	Breakdown Yes/No	Deterioration Yes/No	
Supplementary information: Tests conducted under the conditions of 11.1, in ME EQUIPMENT or under simulated conditions on the bench. See Clause 15.5.2 for test parameters & other details Switch mode transformer incorporated within the power supply unit.						

16.1	RM RESULTS TABLE: General requirements for ME Systems			N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks		Verdict
4.2				
4.3				

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
16.1	RM RESULTS TABLE: General requirements for ME Systems		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.4			
5			
Supplementary information: /			

16.6.1	TABLE: LEAKAGE CURRENTS in ME SYSTEM _ TOUCH CURRENT MEASUREMENTS				N/A
Specific area where TOUCH CURRENT measured (i.e., from or between parts of ME SYSTEM within PATIENT ENVIRONMENT)	Allowable TOUCH CURRENT in NORMAL CONDITION (μA)	Measured TOUCH CURRENT in NORMAL CONDITION (μA)	Allowable TOUCH CURRENT in event of interruption of PROTECTIVE EARTH CONDUCTOR, (μA)	Measured TOUCH CURRENT in event of interruption of PROTECTIVE EARTH CONDUCTOR, (μA)	
	100		500		
	100		500		
	100		500		
	100		500		
	100		500		
Supplementary information: /					

16.9.1	RM RESULTS TABLE: Connection terminals and connectors		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

17	RM RESULTS TABLE: Electromagnetic compatibility of ME equipment and ME systems		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.2			
4.3			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict
17	RM RESULTS TABLE: Electromagnetic compatibility of ME equipment and ME systems		N/A
Clause of ISO 14971	Document Ref. in RMF (Document No. & paragraph)	Result - Remarks	Verdict
4.4			
5			
6.2			
6.3			
6.4			
6.5			
Supplementary information: /			

SP	TABLE: Additional or special tests conducted		P
Clause and Name of Test	Test type and condition	Observed results	
Supplementary information:			
See table on next page			

IEC 60601-1			
Clause	Requirement + Test	Result - Remark	Verdict

--	TABLE: evaluation of voltage limiting components in SELV circuits			P
Component (measured between)		max. voltage (V) (normal operation)		Voltage Limiting Components
		V peak	V d.c.	
Model: GTM2065-8048-FA				
Transformer T1 (Pin 7,8 to Pin 10,11)	352 Vpeak / 92,5 Vrms	--	D101	
Transformer T1 (Pin 7,8 to D101 Cathode)	52 Vpeak / 47,6 Vrms	--	L100	
Transformer T1 (Pin 7,8 to L100 out)	49,6	47,7	SELV	
Model: GTM2065-8036-FA				
Transformer T1 (Pin 7,8 to Pin 10,11)	273 Vpeak / 72,6 Vrms	--	Diode D101	
Transformer T1 (Pin 7,8 to D101 Cathode)	40 Vpeak/ 35,5 Vrms	--	SELV	
Model: GTM2065-8024-FA				
Transformer T1 (Pin 7,8 to Pin 10,11)	132 Vpeak / 46,9 Vrms	--	Diode D101	
Transformer T1 (Pin 7,8 to D101 Cathode)	29 Vpeak/ 24,0 Vrms	--	SELV	
Supplementary information: /				

Enclosure No. 1

National Differences to IEC 60601-1:2005

(13 pages including this cover page)

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict

US NATIONAL DIFFERENCES to IEC 60601-1 Third edition National standard ANSI/AAMI ES60601-1: 2005			
4.8	Components of ME EQUIPMENT	--	P
	When no relevant US ANSI standard existed, the requirements of this standard applied	Considered.	P
4.10.2.	SUPPLY MAINS for ME EQUIPMENT and ME SYSTEMS	--	P
	Replacement: Reference to "500 V" replaced with "600 V" in the second and third dashes to agree with the National Electrical Code (NEC) "and the NEC" added after the reference to "IEC 60364-4-41" in the text of the second-to-last dash of this sub-clause to agree with NEC	Considered.	P
8.2	Requirements related to power sources	--	N/A
	Addition to agree with NEC: The requirement, "ALL FIXED ME EQUIPMENT and PERMANENTLY INSTALLED ME EQUIPMENT are CLASS I ME EQUIPMENT"	EUT is not permanently installed equipment or fixed ME equipment.	N/A
8.7.3	Allowable values:	--	P
	Deleted the second sentence and note to sub-clause 8.7.3 d) to read as follows to agree with NFPA 99 which does not permit for allowances larger than the stated values:	--	P
	d) The allowable values of the EARTH LEAKAGE CURRENT are 5 mA in NORMAL CONDITION and 10 mA in SINGLE FAULT CONDITION	Considered.	P
8.11.	MAINS PARTS, components and layout	--	N/A
	Addition to agree with NEC:	--	N/A
	The requirement, "Permanently connected ME EQUIPMENT shall have provision for the connection of one of the wiring systems that is in accordance with the NEC" Fixed and stationary X-ray ME EQUIPMENT supplied from a branch circuit rated at 30 A or less, and ME EQUIPMENT not strictly portable but obviously intended to be stationary, considered acceptable when supply connection provided with a length of attached Type S hard service flexible cord, or equivalent:	EUT is not permanently connected equipment.	N/A
	Installation of connecting cords between EQUIPMENT parts comply with NEC, as applicable	No connecting cord between equipment parts provided. Only output cable provided.	N/A

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	<p>Cable used as external interconnection between units was:</p> <p>1) Type SJT, SJTO, SJO, ST, SO, STO, or equivalent flexible cord when exposed to abuse, or similar multiple-conductor appliance-wiring material such as computer cable:</p> <p>2) The cable was as in item 1) above when not exposed to abuse, or it was</p> <p style="padding-left: 40px;">i) Type SPT-2, SP-2, or SPE-2, or equivalent</p> <p style="padding-left: 40px;">ii) Type SVr, SVRO, SVE, or equivalent flexible cord or similar multiple-conductor appliance wiring material,</p> <p style="padding-left: 40px;">Or, ii) An assembly of insulated wires each with a nominal insulation thickness of 0.8 mm (1/32 inch) or more, enclosed in acceptable insulating tubing having a nominal wall thickness of 0.8 mm (1/32 inch) or more.</p>	--	N/A
	Receptacles provided as part of ME EQUIPMENT or ME SYSTEMS for use in the patient care areas of pediatric wards, rooms, or areas are listed (e.g., UL Certified) tamper resistant or employ a listed (e.g., UL Certified) tamper resistant cover in accordance with NEC	--	N/A
8.11.3.2.	Addition to agree with NEC:	Power supply cord was not part of the investigation.	N/A
	The flexible cord is a type acceptable for the particular application, and it is acceptable for use at a voltage not less than the rated voltage of the appliance and has an ampacity as in NEC, not less than the current rating of the appliance.	--	N/A
CANADA NATIONAL DIFFERENCES to IEC 60601-1 Third edition National standard CAN/CSA-C22.2 No. 60601-1:08			
1.1	Scope	--	P

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	<p>This standard applies to the BASIC SAFETY and ESSENTIAL PERFORMANCE of MEDICAL ELECTRICAL EQUIPMENT and MEDICAL ELECTRICAL SYSTEMS designed to be installed in accordance with the Canadian Electrical Code (CEC), Part I, CSA C22.1; CAN/CSA-C22.2 No. 0; and CAN/CSA-Z32.</p> <p>NOTE 1A: In the IEC 60601 standards series adopted for use in Canada, the Canadian-particular standards may modify, replace, or delete requirements contained in this standard as appropriate for the particular ME EQUIPMENT and ME SYSTEMS under consideration, and may add other BASIC SAFETY and ESSENTIAL PERFORMANCE requirements.</p>	Considered.	P
1.3	Collateral standards	--	P
	<p>Applicable Canadian collateral standards become normative at the date of their publication and apply together with this standard.</p> <p>NOTE 1: When evaluating compliance with CAN/CSA-C22.2 No. 60601-1, it is permissible to assess independently compliance with the adopted Canadian collateral standards</p>	Considered.	P
1.4	Particular standards	--	P
	A requirement of a Canadian-particular safety standard takes precedence over this standard.	Considered.	P
2	<p>Normative references</p> <p>The following referenced documents are indispensable for the application of this document.</p> <p>For dated references, the applicable corresponding Canadian adopted IEC standards shall take precedence. For undated references, the latest edition of the referenced document (including any amendments) applies. All Canadian adopted IEC part 2 standards are referenced with the date of publication.</p>	Considered.	P

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	<p>CSA (Canadian Standards Association)</p> <p>B51-03: Boiler, pressure vessel, and pressure piping code</p> <p>C22.1-06: Canadian Electrical Code, Part I</p> <p>CAN/CSA-C22.2 No. 0-M91 (R2006): General requirements — Canadian Electrical Code, Part II</p> <p>C22.2 No. 21-95 (R2004): Cord sets and power supply cords</p> <p>C22.2 No. 42-99 (R2004): General use receptacles, attachment plugs, and similar wiring devices</p> <p>C22.2 No. 49-06: Flexible cords and cables</p> <p>CAN/CSA-E61558-2-1:03: Safety of power transformers, power supply units and similar — Part 2: Particular requirements for separating transformers for general use</p> <p>CAN/CSA-Z32-04: Electrical safety and essential electrical systems in health care facilities</p>	Considered.	P

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	Z305 series of Standards: CAN/CSA-Z305.1-92 (R2001): Non-flammable medical gas piping systems CAN/CSA-Z305.6-92 (R2007): Medical oxygen concentrator central supply system for use with non-flammable medical gas piping systems CAN/CSA-Z305.8-03. Medical supply units CAN/CSA-Z305.12-98 (R2004): Guide for the safe storage, handling and use of portable oxygen systems in home, domiciliary and healthcare settings CAN/CSA-Z5359-04: Low pressure hose assemblies for use with medical gases CAN/CSA-Z9170-1-00 (R2005): Terminal units for medical gas pipeline systems — Part 1: Terminal units for use with compressed medical gases and vacuum CAN/CSA-Z9170-2-00 (R2005): Terminal units for medical gas pipeline systems — Part 2: Terminal units for anaesthetic gas scavenging systems CAN/CSA-Z9170-2-00 (R2005): Terminal units for medical gas pipeline systems — Part 2: Terminal units for anaesthetic gas scavenging systems CAN/CSA-Z15002-02 (R2007): Flow-metering devices for connection to terminal units of medical gas pipeline systems ASME International (American Society of Mechanical Engineers) PTC 25-2001: Pressure Relief Devices CGA (Compressed Gas Association): V-1-2005: Standard for Compressed Gas Cylinder Valve Outlet and Inlet Connections V-5-2005: Diameter Index Safety System (Non interchangeable Low Pressure Connections for Medical Gas Applications)	Considered.	P
	ISO (International Organization for Standardization) 32:1977: Gas cylinders for medical use — Marking for identification of content 407:2004: Small medical gas cylinders — Pin-index yoke-type valve connections	--	N/A
3.41	HIGH VOLTAGE	--	N/A

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	any voltage above 750 V, 1 050 V peak, as defined in the Canadian Electrical Code (CEC), Part I	No such high voltage within the equipment.	N/A
4.8	Components of ME EQUIPMENT	--	P
	a) the applicable safety requirements of a relevant CSA, IEC, or ISO standard; NOTE 1: For the components, it is not necessary to carry out identical or equivalent tests already performed to check compliance with the component standard.	Considered.	P
	b) where there is no relevant CSA, IEC, or ISO standard, the requirements of this standard have to be applied NOTE 2: If there are neither requirements in this standard nor in a CSA, IEC, or ISO standard, any other applicable source (e.g., standards for other types of devices, national standards) could be used to demonstrate compliance with the RISK MANAGEMENT PROCESS.	Considered.	P
4.10.2	SUPPLY MAINS for ME EQUIPMENT and ME SYSTEMS	--	P
	and shall be in accordance with the Canadian Electrical Code (CEC), Part I, CSA C22.1:	--	P
7.7.1 to 7.7.5	A PROTECTIVE EARTH CONDUCTOR or a PROTECTIVE EARTH CONNECTION or insulation shall be identified by either green or green and yellow colour. Colours of neutral and POWER SUPPLY CORD conductors shall be in accordance with the Canadian Electrical Code (CEC), Part I, CSA C22.2 No. 21, and CSA C22.2 No. 49.	See enclosed pictures of the unit for details.	P
8.7.3	Allowable values Allowable values shall be in accordance with the Canadian Electrical Code (CEC), Part I, CSA C22.1.	Considered.	P
8.11.3.2	POWER SUPPLY CORDS Types	--	N/A

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	<p>a) The MAINS PLUG of non-PERMANENTLY INSTALLED EQUIPMENT shall be</p> <p>i) if molded-on type, hospital grade mains plug complying with CSA C22.2 No. 21;</p> <p>j) hospital grade disassembly attachment plug type complying with CSA C22.2 No. 42; or</p> <p>k) Class II equipment having fuses on the line side/sides and neutral and may use a non-polarized attachment plug or a polarized attachment plug — CSA configuration type 1-15P shall be required and shall meet all applicable requirements in CSA C22.2 No. 21 and CSA C22.2 No. 42. Where a polarized attachment plug is used, the POWER SUPPLY CORD shall be connected to the wiring of the EQUIPMENT on the ungrounded side of the line when any of the following devices are used in the primary circuit:</p> <p>1- the centre contact of an Edison base lamp holder;</p> <p>2- a single pole switch;</p> <p>3- an automatic control with a marked off position;</p> <p>4- a solitary fuse/fuse holder; or</p> <p>5- any other single pole over-current protective device</p>	Power supply cord was not part of the investigation.	N/A
	<p>b) Detachable POWER SUPPLY CORD for non-PERMANENTLY INSTALLED EQUIPMENT (cord-connected equipment) shall be of a type that</p> <p>i) can be shown to be unlikely to become detached accidentally, unless it can be shown that detachment will not constitute a safety HAZARD to a PATIENT or OPERATOR;</p> <p>j) can be shown that the impedance of the earth (ground) circuit contacts will not constitute a safety HAZARD to a PATIENT or OPERATOR; and</p> <p>k) has a terminal configuration or other constructional feature that will minimize the possibility of its replacement by a detachable POWER SUPPLY CORD which could create a HAZARDOUS SITUATION</p>	Power supply cord was not part of the investigation.	N/A

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	<p>c) A detachable POWER SUPPLY CORD shall</p> <p>i) comply with the applicable requirements of CSA C22.2 No. 21; and</p> <p>j) not be smaller than No. 18 AWG, and the mechanical serviceability shall be not less than</p> <p>1) Type SJ or equivalent for mobile or exposed to abuse ME EQUIPMENT; and</p> <p>2) Type SV or equivalent for ME EQUIPMENT not exposed to abuse (or Type HPN if required because of temperature).</p> <p>NOTE 1A: See CSA C22.2 No. 49 for requirements on the cord types mentioned in Sub-item 2).</p>	Power supply cord was not part of the investigation.	N/A
	<p>d) Power supply cords shall meet the requirements of the Canadian Electrical Code, Part I, as applicable.</p> <p>Connecting cords between equipment parts shall meet the requirements of the Canadian Electrical Code, Part I, as applicable.</p>	Power supply cord was not part of the investigation.	N/A
8.11.5	<p>Mains fuses and OVER-CURRENT RELEASES</p> <p>Mains fuses and OVER-CURRENT RELEASES shall be in accordance with the Canadian Electrical Code (CEC), Part I, CSA C22.1.</p>	See list of critical components.	P
9.7.5	<p>Pressure vessels</p> <p>Pressure vessels shall comply with the requirements of CSA B51, as applicable.</p>	No pressure vessels provided.	N/A
9.7.7	<p>Pressure-relief device</p> <p>A pressure-relief device shall also comply as applicable to the requirements of ASME PTC 25 or equivalent Canadian requirements.</p>	No pressure-relief devices provided.	N/A

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
15.4.1	<p>Construction of connectors</p> <p>The point of connection of gas cylinders to EQUIPMENT shall be gas specific and clearly identified so that errors are avoided when a replacement is made. Medical gas inlet connectors on EQUIPMENT shall be</p> <p>i) gas specific, yoke type, or nut and nipple type valve connections complying with CGA V-1 for pressures over 1 380 kPa (200 psi); or</p> <p>DISS type complying with CGA V-5 for pressures 1 380 kPa (200 psi) or less and configured to permit the supply of medical gases from low-pressure connecting assemblies complying with CAN/CSA-Z5359.</p> <p>NOTE 1A: Users of this standard should consult the CSA Z305 series of standards, CAN/CSA-Z9170-1, CAN/CSA-Z9170-2, CAN/CSA-Z10524, and CAN/CSA-Z15002 for further information regarding inlet connectors; ISO 407 for requirements addressing yoke-type valve connections; and ISO 32 for colour coding.</p>	No gas cylinders provided.	N/A
15.4.8	<p>Internal wiring of ME EQUIPMENT</p> <p>Internal wiring of ME EQUIPMENT shall be in accordance with the Canadian Electrical Code (CEC), Part I, CSA C22.1.</p>	--	P
16.1	<p>MULTIPLE SOCKET OUTLET</p> <p>The MULTIPLE SOCKET-OUTLET shall comply with the requirements of CSA C22.2 No. 42, CSA C22.2 No. 49, and the following requirements.</p> <ul style="list-style-type: none"> - The separating transformer shall comply with the requirements of CAN/CSA-E61558-2-1 with a rated output not exceeding - 1 kVA for single-phase transformers; and - 5 kVA for polyphase transformers <p>The separating transformer shall also have a degree of protection not exceeding IPX4.</p>	No multiple socket outlets provided.	N/A
SWITZERLAND NATIONAL DIFFERENCES to IEC 60601-1 Third edition National standard SN EN 60601-1:06			
4	<p>Ordinance on environmentally hazardous substances SR 814.081, Annex 1.7,</p> <p>Mercury - Annex 1.7 of SR 814.81 applies for mercury.</p>	No mercury used during normal use of the equipment.	N/A

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
	Switches containing mercury such as thermostats, relays and level controllers are not allowed.	No such switched provided.	N/A
	Ordinance on chemical hazardous risk reduction SR 814.81, Annex 2.15: Batteries	--	N/A
	Annex 2.15 of SR 814.81 applies for batteries containing cadmium and mercury.	No batteries incorporated.	N/A
	Note: Ordinance relating to environmentally hazardous substances, SR 814.013 of 1986-06-09 is not longer in force and superseded by SR 814.81 of 2009-02-01 (ChemRRV).	--	N/A
	Supply cords of portable electrical appliances having a rated current not exceeding 10 A shall be provided with a plug complying with IEC 60884-1(3.ed.) + am1, SEV 1011 and one of the following dimension sheets: - SEV 6533-2:2009 Plug type 11, L + N, 250V 10A - SEV 6534-2:2009 Plug type 12, L + N + PE, 250V 10A - SEV 6532-2:2009 Plug type 15, 3L + N + PE, 250/400V 10A	Power supply cord was not part of the investigation.	N/A
4	Supply cords of portable electrical appliances having a rated current not exceeding 16 A shall be provided with a plug complying with IEC 60884-1(3.ed.) + am1, SEV 1011 and one of the following dimension sheets: - SEV 5933-2:2009 Plug type 21 L + N, 250 V, 16A - SEV 5934-2:2009 Plug type 23 L + N + PE, 250 V, 16A - SEV 5932-2:2009 Plug type 25 3L + N + PE, 250/400V 16A	Power supply cord was not part of the investigation.	N/A
	NOTE 16 A plugs are not often used in Swiss domestic installation system.	--	N/A
	See TRF template regulatory requirements Switzerland on IECEE Website R.R. TRF templates.	--	N/A
EU DIFFERENCES			
Standard: EN 60601-1:2006/A11:2011			
ZZ	Replace Annex ZZ of EN 60601-1:2006 by:	--	P

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
ZZA	<p>Annex ZZA (informative) EN 60601-1 :2006/A 11 :2011 Coverage of Essential Requirements of EC Directives This European Standard has been prepared under a mandate given to CENELEC by the European Commission and the European Free Trade Association and within its scope the standard covers all relevant essential requirements as given in Annex I of the EC Directive 93/42/EEC except the following: Essential Requirement 6a Essential Requirement 7.4 Essential Requirement 7.5 paragraph 2 & 3 Essential Requirement 13.6 (q) Compliance with this standard provides one means of conformity with the specified essential requirements of the Directives concerned. WARNING: Other requirements and other EC Directives may be applicable to the products falling within the scope of this standard.</p>	Considered.	P

National Differences			
Clause	Requirement + Test	Result - Remark	Verdict
ZZB	<p>Annex ZZB (informative)</p> <p>Coverage of Essential Requirements of EC Directives</p> <p>This European Standard has been prepared under a mandate given to CENELEC by the European Commission and the European Free Trade Association and within its scope the standard covers all relevant essential requirements as given in Annex I of the EC Directive 90/385/EEC except the following:</p> <p>Essential Requirement 5a Essential Requirement 7 Essential Requirement 8 bullet 5 Essential Requirement 10 Essential Requirement 11 Essential Requirement 12 Essential Requirement 14 Essential Requirement 15 Essential Requirement 16</p> <p>Compliance with this standard provides one means of conformity with the specified essential requirements of the Directives concerned.</p> <p>WARNING: Other requirements and other EC Directives may be applicable to the products falling within the scope of this standard.</p>	Considered.	P

Enclosure No. 2

Photo documentation

(4 pages including this cover page)

